

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050324\
 Data File : VV035527.D
 Acq On : 03 May 2024 10:54
 Operator : SY/MD
 Sample : P2349-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

Signal : TIC: VV035527.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	93	rVB	215400	234904	14.19%	1.865%
2	1.529	145	152	171	rVB	201460	238425	14.40%	1.893%
3	2.056	306	316	334	rBV	376183	540495	32.65%	4.291%
4	2.236	369	372	379	rVB3	1088	1312	0.08%	0.010%
5	2.336	400	403	409	rBV4	448	483	0.03%	0.004%
6	2.400	420	423	424	rBV2	436	267	0.02%	0.002%
7	2.439	430	435	446	rBV8	1745	2810	0.17%	0.022%
8	2.513	454	458	460	rVB2	290	240	0.01%	0.002%
9	2.532	460	464	466	rBV2	344	246	0.01%	0.002%
10	2.703	513	517	520	rBV5	478	293	0.02%	0.002%
11	2.728	522	525	528	rVB2	351	266	0.02%	0.002%
12	2.754	528	533	536	rBV2	251	211	0.01%	0.002%
13	2.786	536	543	544	rBV2	262	284	0.02%	0.002%
14	2.828	554	556	561	rVB3	294	209	0.01%	0.002%
15	2.950	590	594	598	rVB3	234	219	0.01%	0.002%
16	2.986	600	605	609	rVB3	396	373	0.02%	0.003%
17	3.786	845	854	900	rBV	130705	387939	23.43%	3.080%
18	4.246	980	997	1026	rBV	264954	688631	41.60%	5.468%
19	4.590	1102	1104	1109	rVB2	461	384	0.02%	0.003%
20	4.616	1109	1112	1115	rBV2	463	399	0.02%	0.003%
21	4.699	1135	1138	1146	rVB2	462	563	0.03%	0.004%
22	4.741	1146	1151	1153	rBV3	459	366	0.02%	0.003%
23	4.777	1161	1162	1166	rVB3	285	207	0.01%	0.002%
24	4.806	1166	1171	1174	rBV2	319	333	0.02%	0.003%
25	4.847	1178	1184	1188	rBV3	404	481	0.03%	0.004%
26	4.953	1200	1217	1253	rBV2	628813	1655421	100.00%	13.144%
27	5.297	1321	1324	1326	rBV3	408	223	0.01%	0.002%
28	5.355	1337	1342	1345	rBV3	505	396	0.02%	0.003%
29	5.432	1362	1366	1370	rBV5	599	650	0.04%	0.005%
30	5.532	1386	1397	1441	rBV	455299	969120	58.54%	7.695%
31	5.834	1479	1491	1512	rVB5	8134	19432	1.17%	0.154%
32	5.986	1525	1538	1572	rBV	365352	759815	45.90%	6.033%
33	6.301	1629	1636	1639	rBV3	409	513	0.03%	0.004%
34	6.317	1639	1641	1646	rVB2	579	317	0.02%	0.003%
35	6.342	1646	1649	1651	rBV	316	195	0.01%	0.002%
36	6.410	1667	1670	1673	rVB2	301	227	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050324\
 Data File : VV035527.D
 Acq On : 03 May 2024 10:54
 Operator : SY/MD
 Sample : P2349-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

37	6.468	1685	1688	1692	rVV2	407	212	0.01%	0.002%
38	6.648	1740	1744	1746	rBV3	551	405	0.02%	0.003%
39	6.715	1762	1765	1768	rVB2	376	229	0.01%	0.002%
40	6.912	1813	1826	1859	rBV	176418	347791	21.01%	2.761%
41	7.191	1911	1913	1917	rVB3	299	218	0.01%	0.002%
42	7.243	1917	1929	1963	rBV	693276	1248922	75.44%	9.916%
43	7.551	2017	2025	2052	rBV	126249	239471	14.47%	1.901%
44	7.760	2088	2090	2094	rVB3	593	379	0.02%	0.003%
45	7.799	2098	2102	2103	rBV2	329	218	0.01%	0.002%
46	7.876	2115	2126	2134	rBV4	1692	3386	0.20%	0.027%
47	7.908	2134	2136	2139	rVB	440	261	0.02%	0.002%
48	8.024	2162	2172	2216	rBV	444021	833766	50.37%	6.620%
49	8.355	2273	2275	2276	rBV2	656	241	0.01%	0.002%
50	8.468	2307	2310	2313	rVB3	326	214	0.01%	0.002%
51	8.571	2338	2342	2348	rBV2	726	552	0.03%	0.004%
52	8.783	2396	2408	2446	rBV	736530	1223450	73.91%	9.714%
53	9.091	2502	2504	2506	rBV3	407	215	0.01%	0.002%
54	9.111	2508	2510	2513	rBV3	489	259	0.02%	0.002%
55	9.178	2529	2531	2535	rVB2	707	413	0.02%	0.003%
56	9.204	2535	2539	2541	rBV2	440	284	0.02%	0.002%
57	9.217	2541	2543	2545	rVV2	493	270	0.02%	0.002%
58	9.230	2545	2547	2552	rVB3	558	421	0.03%	0.003%
59	9.259	2552	2556	2559	rBV	425	319	0.02%	0.003%
60	9.686	2686	2689	2692	rVB	403	231	0.01%	0.002%
61	9.870	2742	2746	2747	rBV2	436	295	0.02%	0.002%
62	9.905	2755	2757	2763	rBV3	180	197	0.01%	0.002%
63	9.998	2781	2786	2789	rBV2	262	265	0.02%	0.002%
64	10.050	2797	2802	2806	rBV2	281	230	0.01%	0.002%
65	10.082	2807	2812	2816	rVV3	321	350	0.02%	0.003%
66	10.149	2821	2833	2871	rBV	576619	920718	55.62%	7.310%
67	10.323	2880	2887	2902	rVB8	2445	4028	0.24%	0.032%
68	11.130	3134	3138	3140	rBV3	658	565	0.03%	0.004%
69	11.185	3143	3155	3188	rBV	678515	1090119	65.85%	8.655%
70	11.474	3237	3245	3248	rVB5	442	569	0.03%	0.005%
71	11.558	3259	3271	3300	rBV	729349	1154715	69.75%	9.168%
72	11.799	3344	3346	3351	rVB3	353	227	0.01%	0.002%
73	11.844	3357	3360	3364	rVB2	471	363	0.02%	0.003%
74	11.863	3364	3366	3370	rBV2	309	295	0.02%	0.002%
75	12.024	3411	3416	3420	rBV3	320	308	0.02%	0.002%
76	12.204	3469	3472	3476	rVB2	612	483	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050324\
 Data File : VV035527.D
 Acq On : 03 May 2024 10:54
 Operator : SY/MD
 Sample : P2349-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
 Title : VOC Analysis

77	12.371	3519	3524	3525	rBV2	318	239	0.01%	0.002%
78	12.448	3543	3548	3550	rBV	435	303	0.02%	0.002%
79	12.497	3560	3563	3565	rBV2	318	203	0.01%	0.002%
80	12.596	3588	3594	3595	rBV4	876	597	0.04%	0.005%
81	12.644	3605	3609	3610	rBV2	277	205	0.01%	0.002%
82	12.722	3631	3633	3637	rVB	313	190	0.01%	0.002%
83	12.747	3637	3641	3646	rVB3	311	277	0.02%	0.002%
84	12.898	3683	3688	3691	rBV3	495	427	0.03%	0.003%
85	12.924	3691	3696	3700	rBV4	367	444	0.03%	0.004%
86	13.095	3746	3749	3752	rBV3	408	263	0.02%	0.002%
87	13.159	3765	3769	3772	rBV2	352	304	0.02%	0.002%
88	13.217	3779	3787	3795	rVB5	1657	2571	0.16%	0.020%
89	13.249	3795	3797	3803	rBV	462	356	0.02%	0.003%
90	13.352	3825	3829	3832	rBV2	378	405	0.02%	0.003%
91	13.381	3835	3838	3842	rVB	370	266	0.02%	0.002%
92	13.458	3856	3862	3864	rBV5	1304	1169	0.07%	0.009%
93	13.689	3926	3934	3939	rBV5	1285	1853	0.11%	0.015%
94	13.722	3942	3944	3949	rBV4	272	213	0.01%	0.002%
95	13.873	3988	3991	3993	rBV3	537	292	0.02%	0.002%
96	14.175	4081	4085	4088	rBV2	485	400	0.02%	0.003%
97	14.268	4111	4114	4116	rBV3	363	291	0.02%	0.002%
98	14.464	4173	4175	4177	rBV2	501	292	0.02%	0.002%
99	14.580	4208	4211	4216	rVB4	511	448	0.03%	0.004%
100	14.728	4255	4257	4260	rBV2	476	374	0.02%	0.003%

Sum of corrected areas: 12594885




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050324\
Data File : VV035527.D
Acq On : 03 May 2024 10:54
Operator : SY/MD
Sample : P2349-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

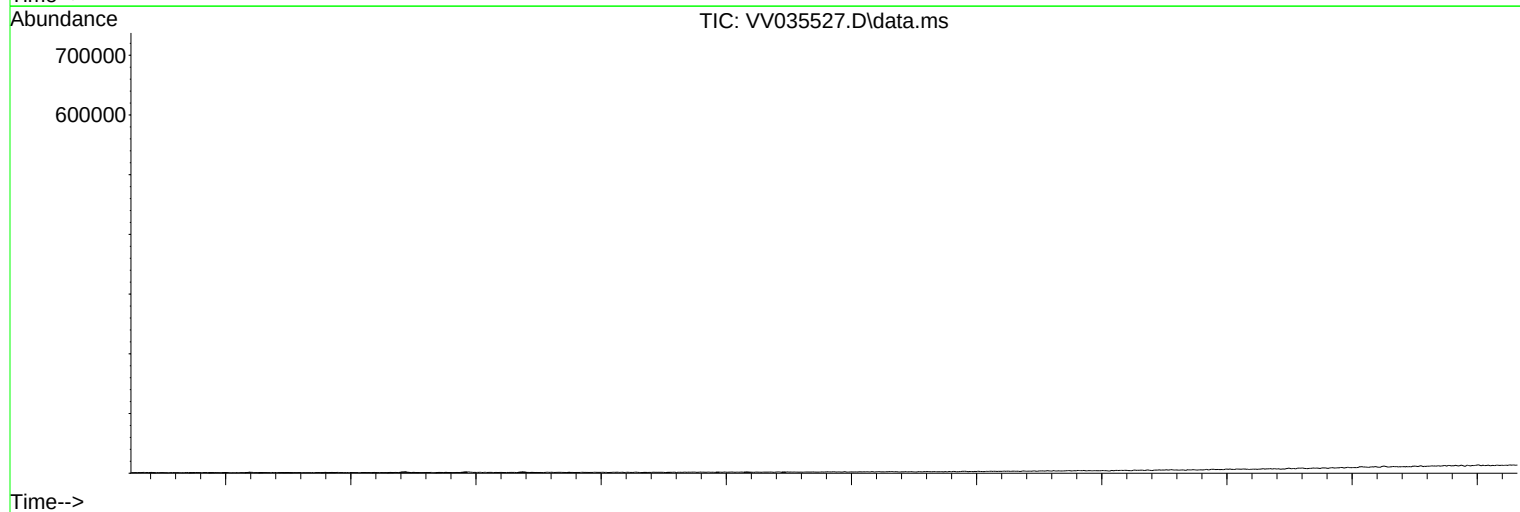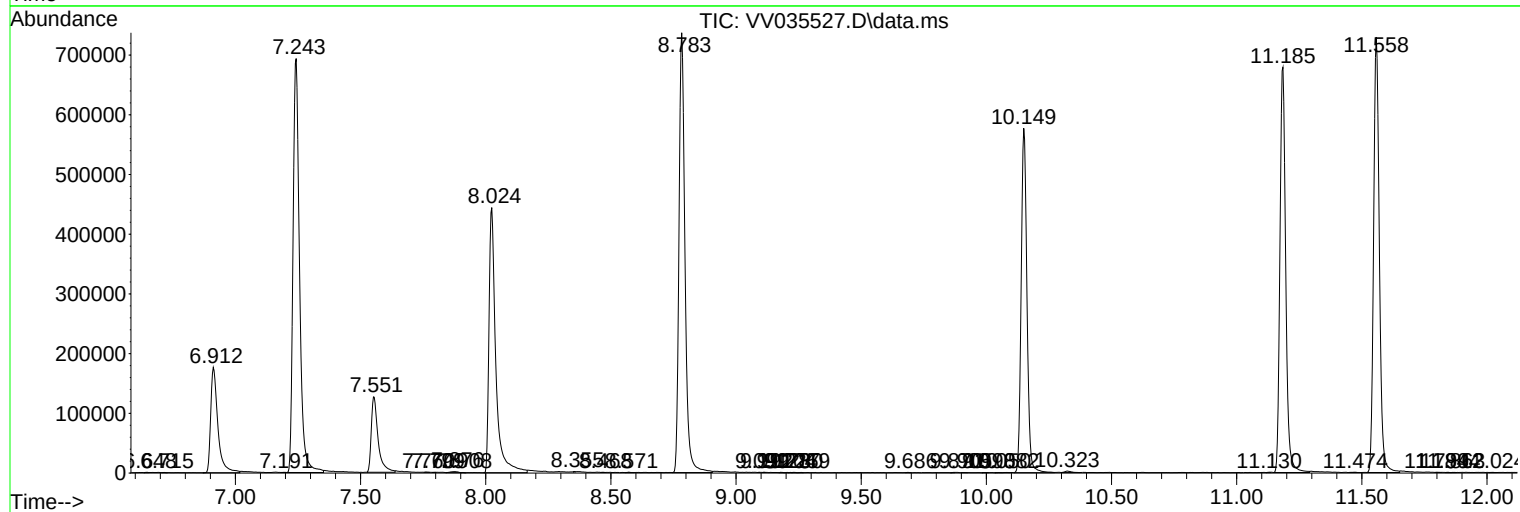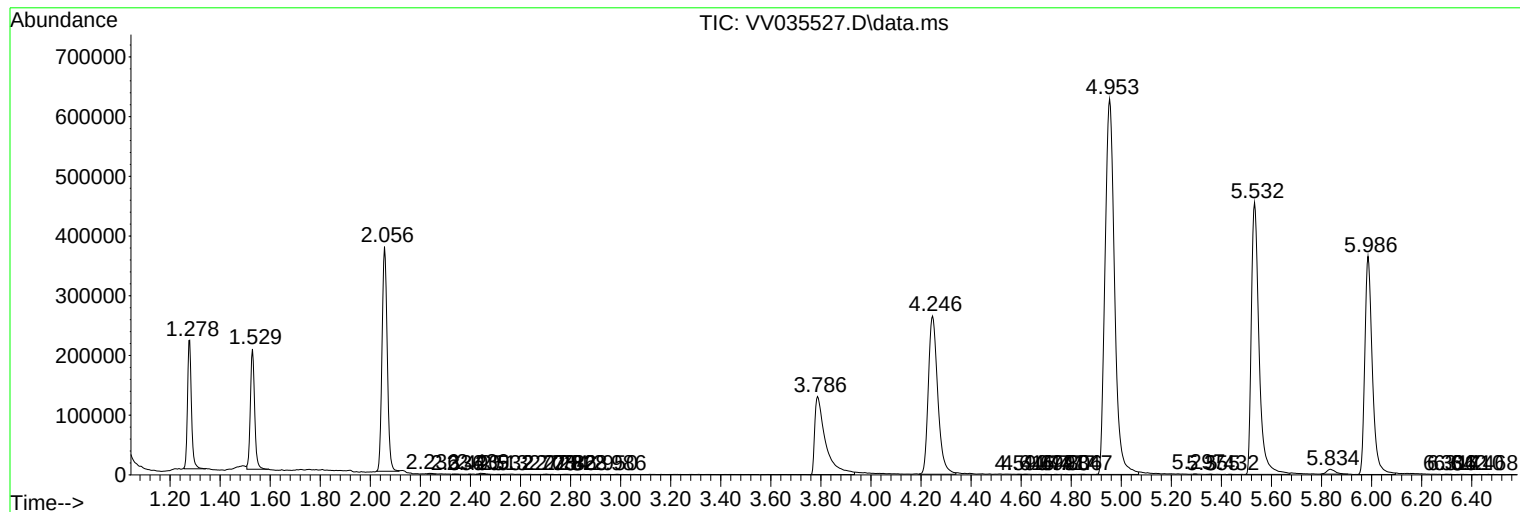

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050324\
Data File : VV035527.D
Acq On : 03 May 2024 10:54
Operator : SY/MD
Sample : P2349-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050324\
Data File : VV035527.D
Acq On : 03 May 2024 10:54
Operator : SY/MD
Sample : P2349-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------