
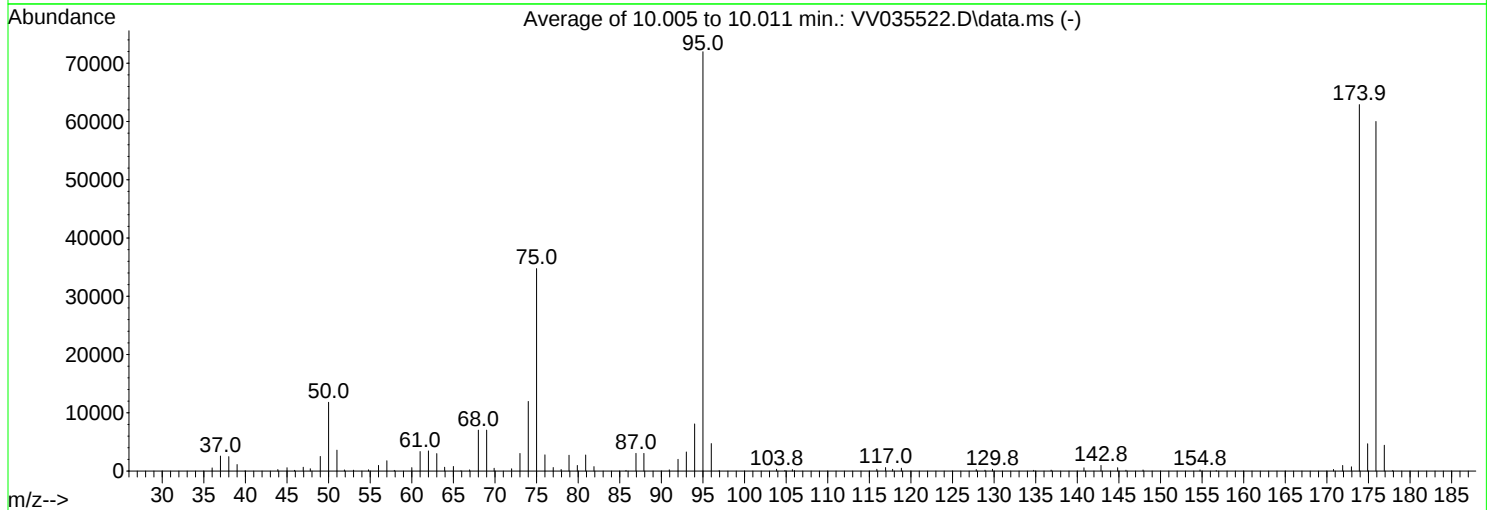


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050324\
Data File : VV035522.D
Acq On : 03 May 2024 08:18
Operator : SY/MD
Sample : BFB296
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB296

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Title : VOC Analysis
Last Update : Mon May 06 13:46:00 2024

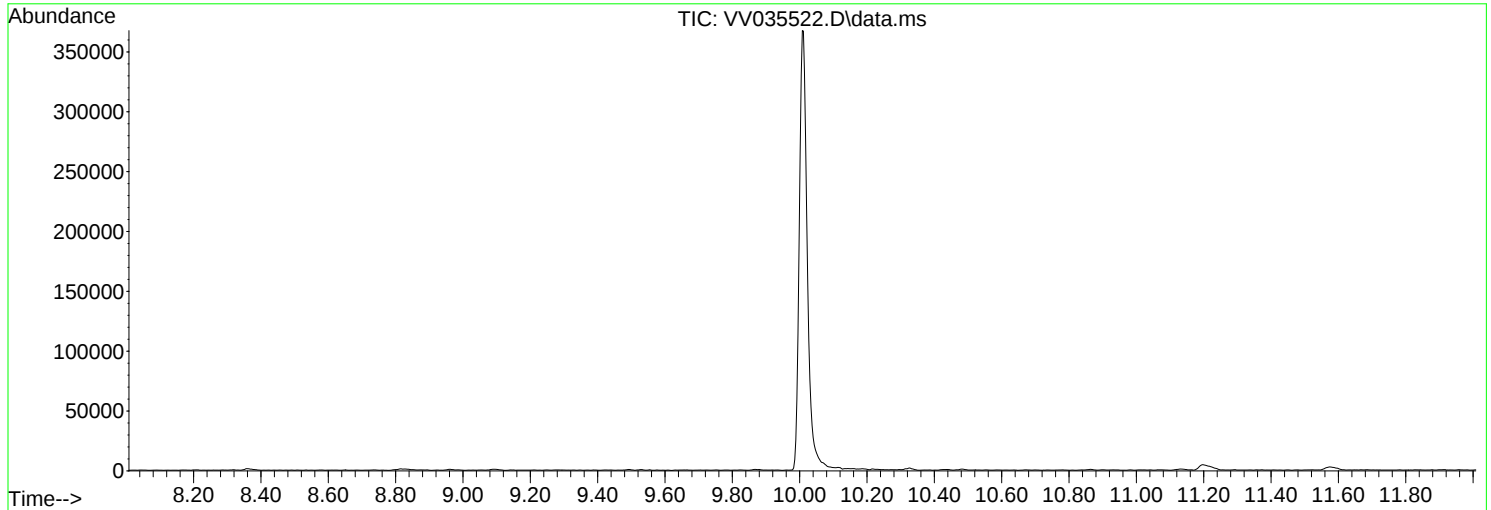

AutoFind: Scans 2788, 2789, 2790; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	11804	PASS
75	95	30	80	48.3	34752	PASS
95	95	100	100	100.0	71971	PASS
96	95	5	9	6.6	4720	PASS
173	174	0.00	2	1.2	734	PASS
174	95	50	120	87.4	62899	PASS
175	174	5	9	7.5	4687	PASS
176	174	95	105	95.4	60003	PASS
177	176	5	10	7.4	4436	PASS

m/z	Abundance
39.90	242.0
43.90	461.0

Instrument :
MSVOA_V
ClientSampleId :
BFB296

m/z	Abundance
36.00	510.0
37.00	2400.0
38.00	2354.0
39.00	1089.0
40.10	253.0
44.00	724.0
45.00	523.0
45.90	158.0
46.90	696.0
47.80	389.0
49.00	2574.0
50.00	10911.0
51.00	3572.0
51.90	169.0
53.00	151.0
54.80	221.0
56.00	943.0
57.00	1604.0
57.90	139.0
60.00	599.0
61.00	3160.0
62.00	3259.0
63.00	2746.0
64.00	652.0
65.00	737.0
67.00	174.0
68.00	6488.0
69.00	6849.0
69.90	417.0
72.00	390.0
73.00	2823.0
74.00	11064.0
75.00	32648.0
76.00	2629.0
77.00	569.0
78.00	256.0
78.90	2585.0
79.90	882.0
80.90	2621.0
81.90	709.0
85.70	101.0
86.90	2754.0
87.90	2979.0
90.90	218.0
92.00	1908.0
93.00	3034.0
94.00	7520.0
95.00	67712.0
96.00	4672.0
96.90	116.0
103.90	300.0
104.90	114.0
105.70	224.0
106.00	223.0
115.90	251.0
117.00	597.0
117.80	253.0
118.80	510.0
127.80	268.0
128.90	153.0
129.80	250.0
134.80	128.0
136.90	185.0
140.80	560.0
142.90	923.0
144.80	554.0
145.90	151.0
147.90	146.0
154.80	178.0
170.80	273.0
171.90	882.0
173.00	642.0
173.90	57192.0
174.90	4534.0
175.90	54824.0
176.90	4094.0

Instrument :
MSVOA_V
ClientSampleId :
BFB296

m/z	Abundance
36.00	587.0
37.00	2702.0
38.00	2578.0
39.00	1176.0
40.10	263.0
43.90	717.0
45.00	582.0
45.90	131.0
47.00	673.0
47.80	426.0
49.00	2648.0
50.00	12259.0
51.00	3701.0
51.90	216.0
53.00	176.0
54.80	234.0
56.00	1026.0
57.00	1815.0
57.90	135.0
60.00	594.0
61.00	3467.0
62.00	3570.0
63.00	3107.0
63.90	678.0
65.00	807.0
67.00	213.0
68.00	7267.0
69.00	7344.0
69.90	487.0
72.00	390.0
73.00	3111.0
74.00	12338.0
75.00	35864.0
76.00	2843.0
77.00	648.0
78.00	285.0
78.90	2872.0
79.90	1007.0
80.90	2868.0
81.90	812.0
85.70	114.0
87.00	3129.0
87.90	3138.0
91.00	221.0
92.00	2112.0
93.00	3398.0
94.00	8357.0
95.00	74464.0
96.00	4890.0
97.00	108.0
103.90	329.0
104.80	124.0
105.70	253.0
115.90	336.0
116.90	624.0
117.80	314.0
118.80	513.0
127.80	265.0
128.90	170.0
129.80	336.0
134.80	137.0
136.80	181.0
140.80	596.0
142.80	980.0
144.90	577.0
145.80	171.0
147.90	200.0
154.80	195.0
156.70	125.0
170.80	295.0
171.90	972.0
173.00	782.0
173.90	65256.0
174.90	4888.0
175.90	61952.0
176.90	4592.0
177.90	110.0

Instrument :
MSVOA_V
ClientSampleId :
BFB296

m/z	Abundance
36.00	550.0
37.00	2636.0
38.00	2517.0
39.00	1105.0
40.00	260.0
43.90	723.0
45.00	636.0
45.90	109.0
47.00	601.0
47.80	395.0
49.00	2325.0
50.00	12241.0
51.00	3505.0
51.90	222.0
53.00	156.0
54.80	221.0
56.00	950.0
57.00	1884.0
57.90	108.0
60.00	589.0
61.00	3435.0
62.00	3560.0
63.00	3151.0
63.90	637.0
65.00	833.0
65.90	109.0
66.90	224.0
68.00	7320.0
69.00	6886.0
69.90	548.0
72.00	408.0
73.00	3135.0
74.00	12455.0
75.00	35744.0
76.00	2894.0
77.00	615.0
77.90	285.0
78.90	2713.0
79.90	1022.0
80.90	2798.0
81.90	786.0
85.80	132.0
86.90	3233.0
87.90	2975.0
91.00	203.0
92.00	2047.0
93.00	3399.0
94.00	8397.0
95.00	73736.0
96.00	4599.0
103.80	337.0
104.90	109.0
105.80	277.0
115.90	357.0
116.90	593.0
117.80	350.0
118.90	471.0
127.90	262.0
128.90	148.0
129.80	361.0
134.70	119.0
136.80	141.0
140.80	544.0
142.80	1033.0
144.90	606.0
145.80	164.0
147.90	227.0
154.70	218.0
156.70	124.0
170.80	262.0
171.90	1054.0
172.90	777.0
173.90	66248.0
174.90	4640.0
175.90	63232.0
176.90	4622.0
177.90	123.0

Instrument :
MSVOA_V
ClientSampleId :
BFB296