

Data Path : W:\HPCHEM1\MSVOA V\DATA\VV050718\
 Data File : VV005827.D
 Acq On : 07 May 2018 19:49
 Operator : SY/MD
 Sample : J2636-12
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1C17

Quant Time: May 08 01:49:09 2018
 Quant Method : W:\HPCHEM1\MSVOA V\METHOD\SOMVTR050518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue May 08 01:22:26 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	246324	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	248845	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	103583	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	85895	4.59	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	91.80%
7) Chloroethane-d5	1.58	69	77273	4.79	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	95.80%
11) 1,1-Dichloroethene-d2	2.13	63	141641	3.43	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.60%
20) 2-Butanone-d5	3.96	46	167590	45.57	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	91.14%
24) Chloroform-d	4.41	84	164258	4.82	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.40%
26) 1,2-Dichloroethane-d4	5.09	65	97720	4.83	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.60%
32) Benzene-d6	5.11	84	308309	4.56	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.20%
36) 1,2-Dichloropropane-d6	6.13	67	93876	4.53	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	90.60%
41) Toluene-d8	7.37	98	274802	4.21	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.20%
43) trans-1,3-Dichloropropene-	7.67	79	34263	4.18	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.60%
46) 2-Hexanone-d5	8.14	63	112452	35.17	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	70.34%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	60267	3.87	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	77.40%
64) 1,2-Dichlorobenzene-d4	11.68	152	100188	4.66	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	93.20%


Target Compounds					Ovalue
13) Acetone	2.20	43	4102	1.32 ug/L	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA V\DATA\VV050718\
Data File : VV005827.D
Acq On : 07 May 2018 19:49
Operator : SY/MD
Sample : J2636-12
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1C17

Quant Time: May 08 01:49:09 2018
Quant Method : W:\HPCHEM1\MSVOA V\METHOD\SOMVTR050518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue May 08 01:22:26 2018
Response via : Initial Calibration

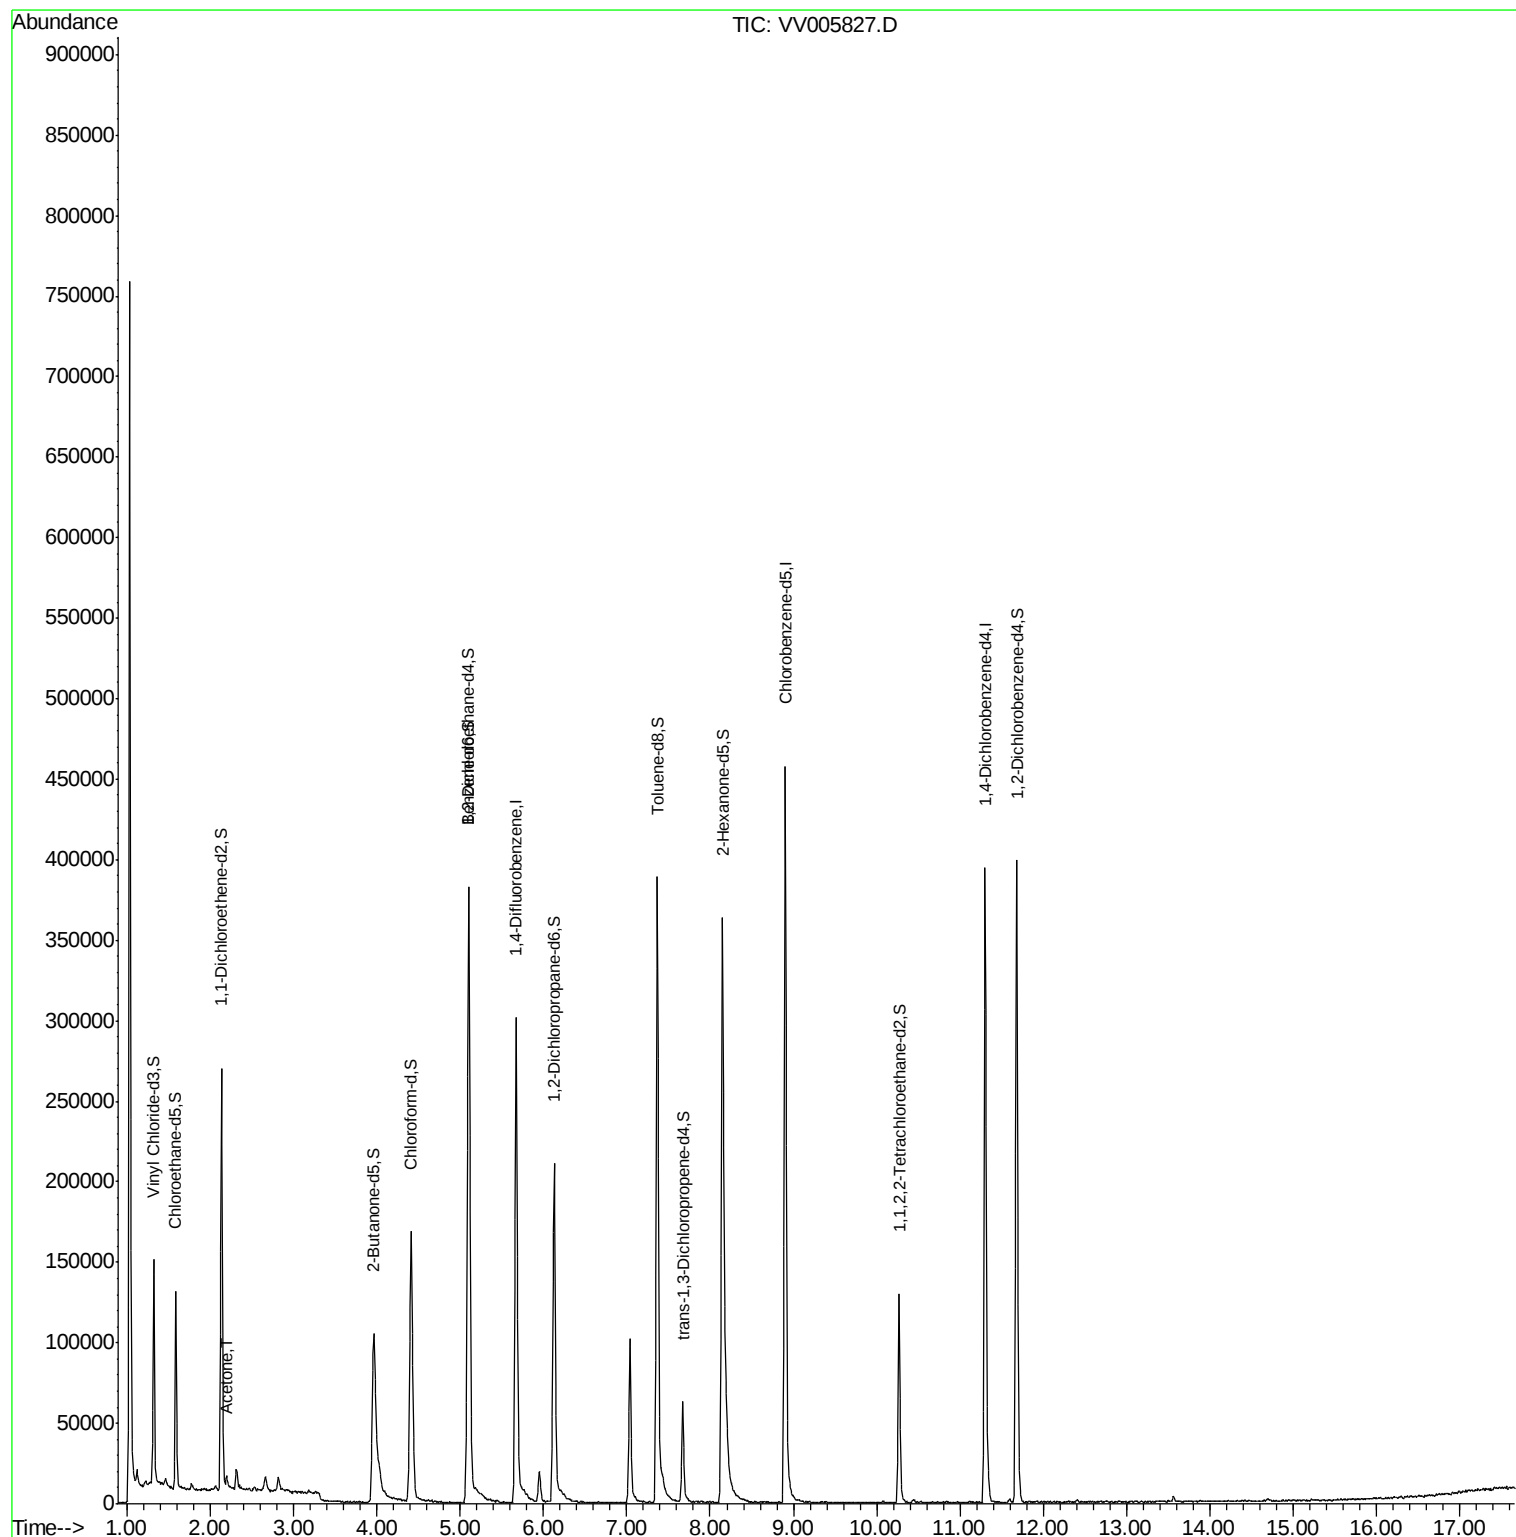

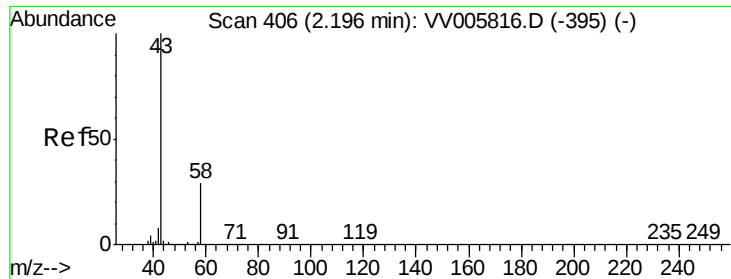

#13
 Acetone
 Concen: 1.32 ug/L
 RT: 2.20 min Scan# 406
 Delta R.T. -0.00 min
 Lab File: VV005827.D
 Acq: 07 May 2018 19:49

Instrument :
 MSVOA_V
 ClientSampleId :
 F1C17

Tot Ion: 43 Resp: 4102
 Ion Ratio Lower Upper
 43 100
 58 36.2 0.0 57.8

