

Data Path : W:\HPCHEM1\MSVOA V\DATA\VV050718\
 Data File : VV005828.D
 Acq On : 07 May 2018 20:16
 Operator : SY/MD
 Sample : J2636-13
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F1C18

Quant Time: May 08 01:50:39 2018
 Quant Method : W:\HPCHEM1\MSVOA V\METHOD\SOMVTR050518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue May 08 01:22:26 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	231007	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	236299	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	96529	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	87150	4.97	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	99.40%
7) Chloroethane-d5	1.58	69	77284	5.11	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	102.20%
11) 1,1-Dichloroethene-d2	2.13	63	142796	3.69	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.80%
20) 2-Butanone-d5	3.96	46	157468	45.65	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	91.30%
24) Chloroform-d	4.41	84	166533	5.21	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.20%
26) 1,2-Dichloroethane-d4	5.09	65	97514	5.14	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.80%
32) Benzene-d6	5.11	84	315629	4.92	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.40%
36) 1,2-Dichloropropane-d6	6.13	67	94301	4.79	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.80%
41) Toluene-d8	7.37	98	277836	4.49	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.80%
43) trans-1,3-Dichloropropene-	7.67	79	33865	4.36	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.20%
46) 2-Hexanone-d5	8.14	63	111519	36.73	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	73.46%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	60887	4.12	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	82.40%
64) 1,2-Dichlorobenzene-d4	11.68	152	100011	4.99	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.80%


Target Compounds					Ovalue
13) Acetone	2.20	43	6400	2.19 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA V\DATA\VV050718\
Data File : VV005828.D
Acq On : 07 May 2018 20:16
Operator : SY/MD
Sample : J2636-13
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F1C18

Quant Time: May 08 01:50:39 2018
Quant Method : W:\HPCHEM1\MSVOA V\METHOD\SOMVTR050518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue May 08 01:22:26 2018
Response via : Initial Calibration

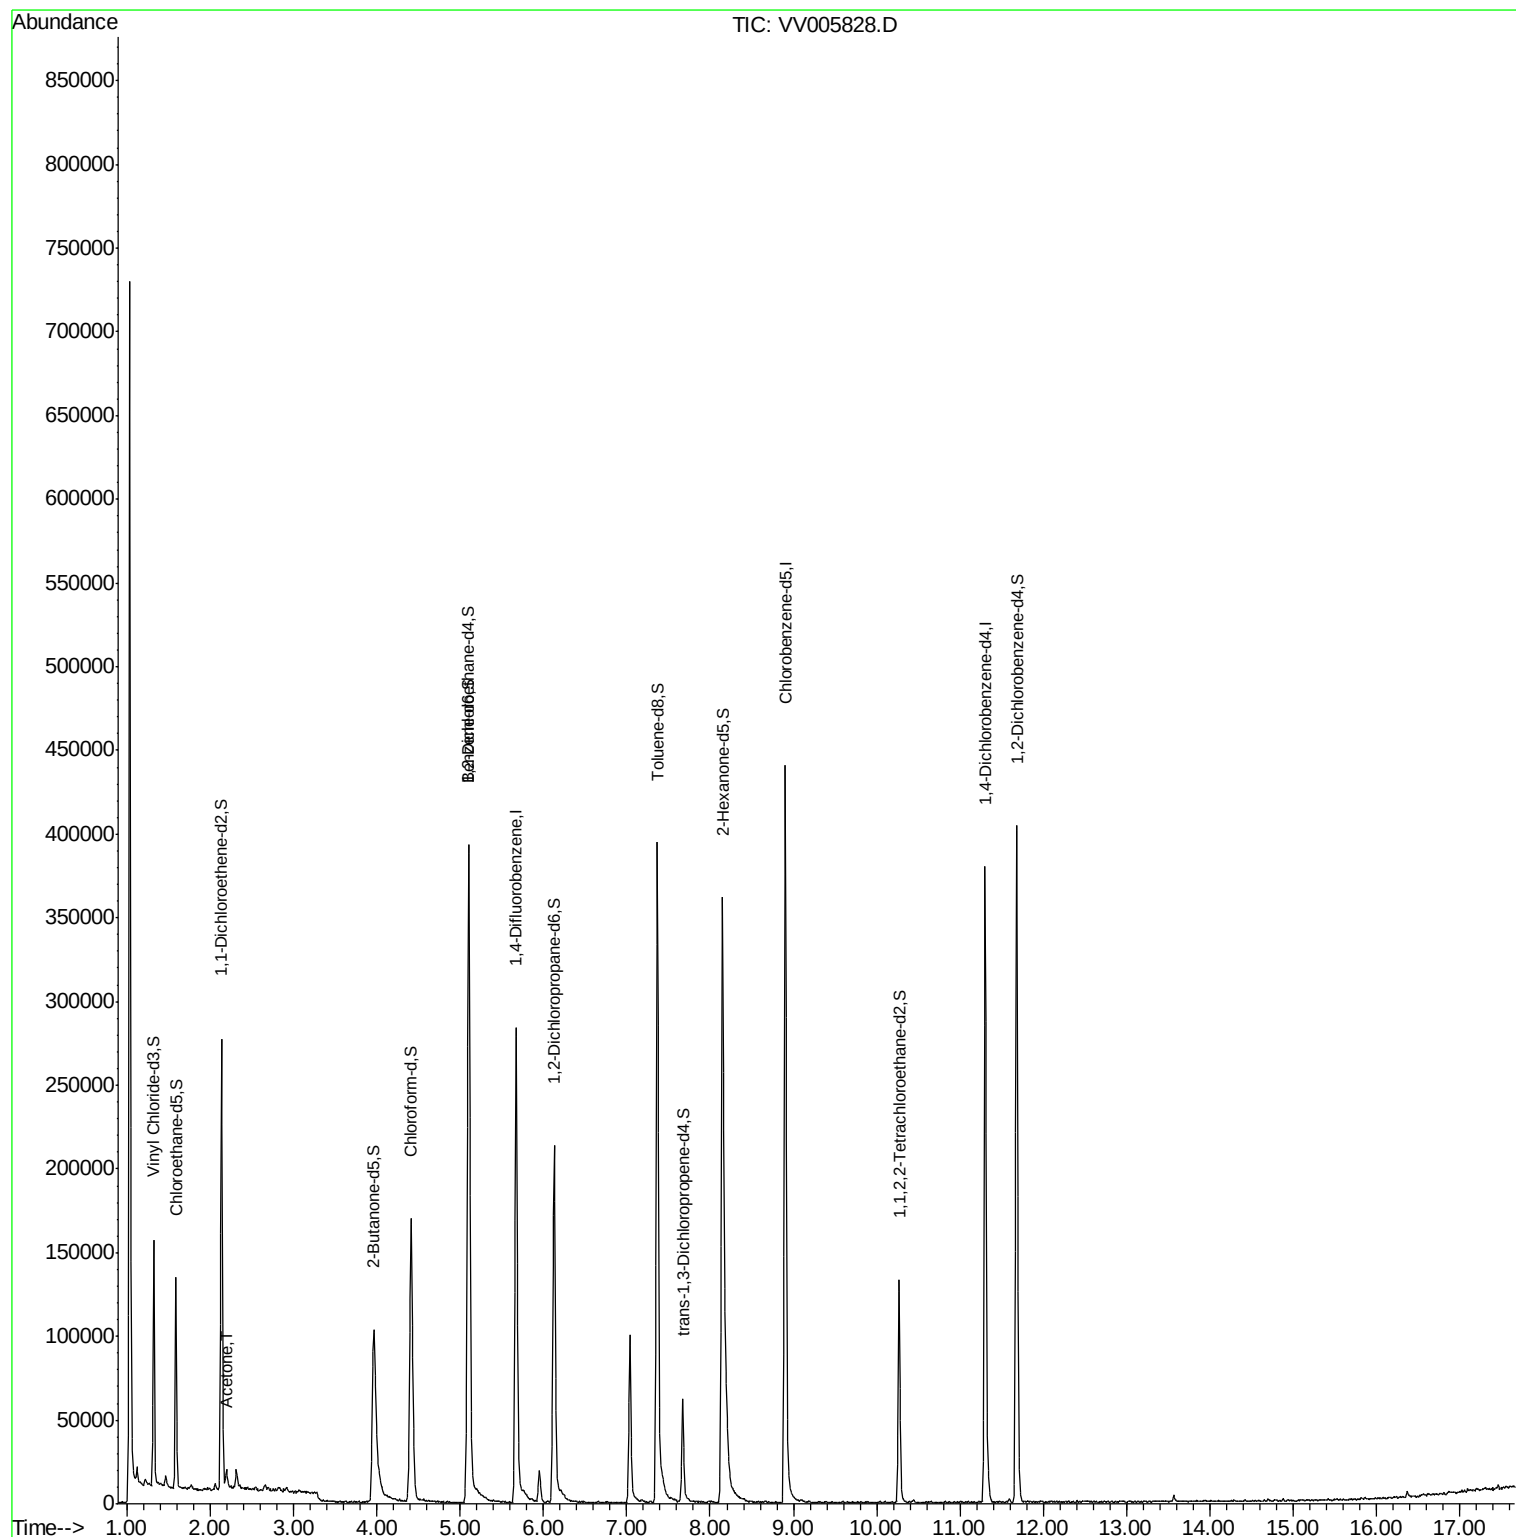

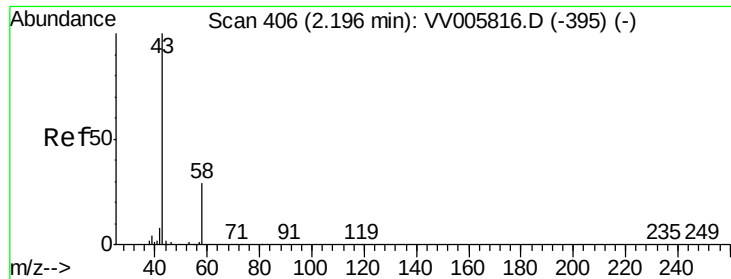

#13
Acetone
Concen: 2.19 ug/L
RT: 2.20 min Scan# 406
Delta R.T. -0.00 min
Lab File: VV005828.D
Acq: 07 May 2018 20:16

Instrument :
MSVOA_V
ClientSampleId :
F1C18

Tot Ion: 43 Resp: 6400
Ion Ratio Lower Upper
43 100
58 29.6 0.0 57.8

