


Data Path : W:\HPCHEM1\MSVOA V\DATA\VV050718\
 Data File : VV005815.D
 Acq On : 07 May 2018 11:07
 Operator : SY/MD
 Sample : BFB74
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB74

Integration File: rteint.p

Method : W:\HPCHEM1\MSVOA_V\METHOD\SOMVTR050518WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Tue May 08 01:22:26 2018

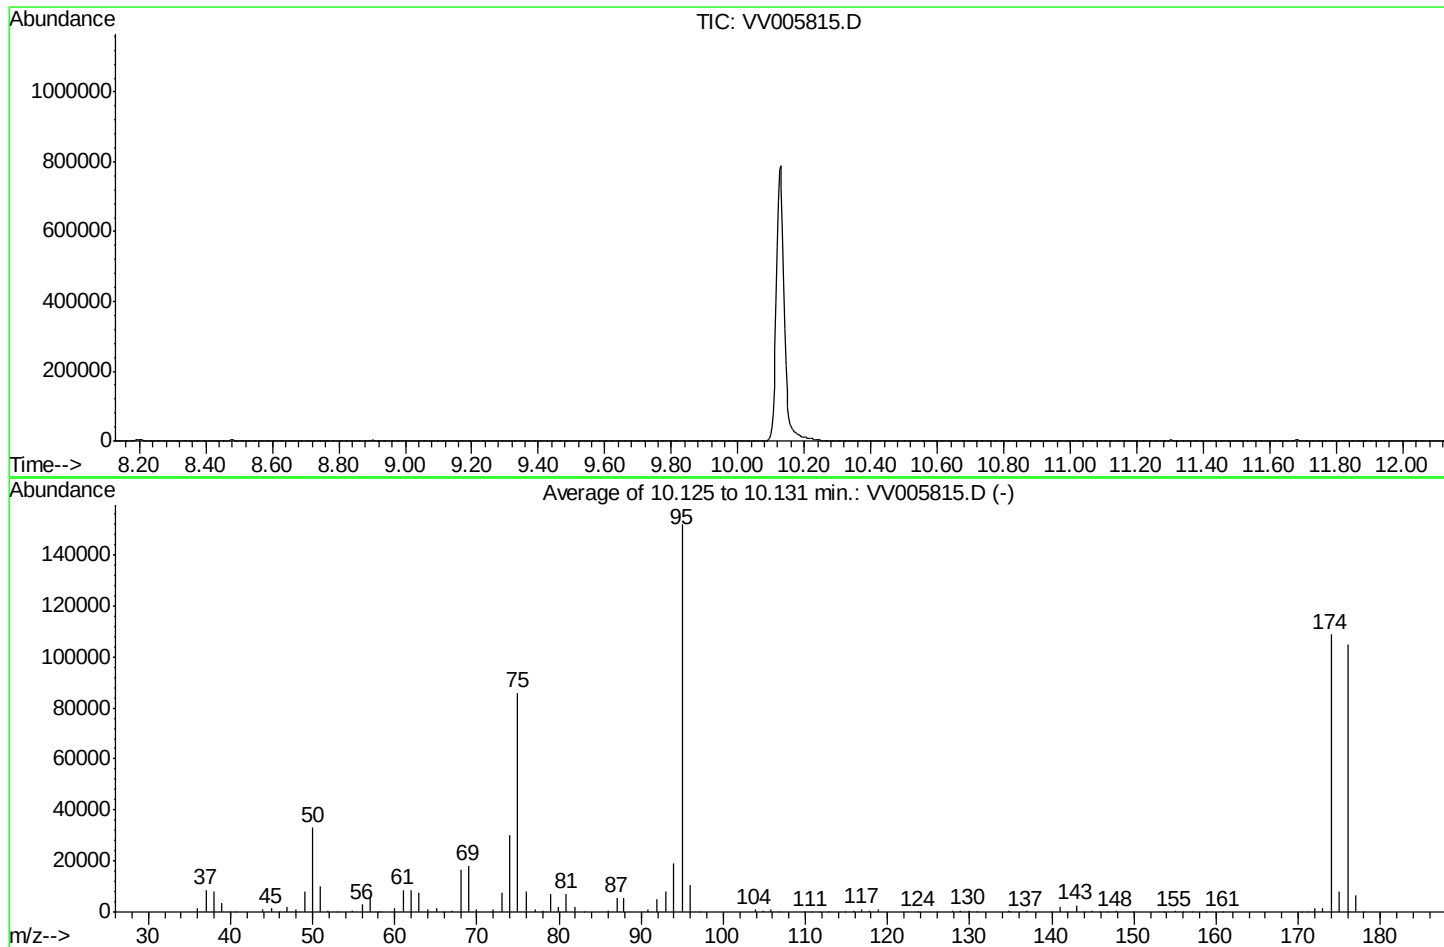

AutoFind: Scans 2872, 2873, 2874; Background Corrected with Scan 2858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.7	33050	PASS
75	95	30	80	56.6	86074	PASS
95	95	100	100	100.0	151978	PASS
96	95	5	9	6.9	10489	PASS
173	174	0.00	2	1.4	1493	PASS
174	95	50	120	71.6	108776	PASS
175	174	5	9	7.5	8154	PASS
176	174	95	101	96.5	105002	PASS
177	176	5	9	6.4	6748	PASS

Scan 2858 (10.080 min): VV005815.D
BFB74

m/z	Abundance
39.80	226.0
43.90	501.0

Instrument :
MSVOA_V
ClientSampleId :
BFB74

m/z	Abundance
36.00	1496.0
37.00	9056.0
38.00	8134.0
39.00	3612.0
39.90	297.0
40.70	131.0
44.00	1459.0
45.00	1362.0
47.00	1859.0
47.90	1171.0
49.00	8365.0
50.00	34624.0
51.00	10050.0
51.90	533.0
53.00	167.0
54.90	427.0
56.00	2814.0
57.00	5668.0
58.20	226.0
59.90	1749.0
61.00	9156.0
62.00	8927.0
63.00	7736.0
64.00	1011.0
65.00	1359.0
65.90	158.0
66.90	528.0
68.00	17040.0
69.00	18568.0
70.00	1298.0
72.00	1161.0
73.00	7934.0
74.00	30872.0
75.00	87664.0
76.00	8329.0
77.10	924.0
78.00	598.0
78.90	7314.0
79.90	1934.0
80.90	7652.0
81.90	1919.0
83.00	266.0
86.00	326.0
87.00	5532.0
87.90	5883.0
90.80	831.0
91.90	4755.0
93.00	8214.0
94.00	19920.0
95.00	156800.0
96.00	10600.0
97.00	287.0
103.90	931.0
105.00	326.0
105.80	1089.0
106.80	181.0
110.00	126.0
110.70	241.0
111.70	195.0
112.90	327.0
114.80	234.0
115.90	614.0
116.80	1241.0
117.80	594.0
118.90	1172.0
123.80	141.0
126.00	104.0
128.00	504.0
128.90	305.0
129.90	775.0
130.90	152.0
134.70	388.0
136.90	313.0
140.00	163.0
141.00	1875.0
141.80	316.0
143.00	2767.0
144.90	534.0
145.90	246.0
146.80	139.0
147.80	514.0
150.00	200.0
153.50	136.0
155.00	371.0
157.00	149.0
158.80	275.0
160.80	131.0
171.10	224.0
172.00	1647.0
173.00	1397.0
174.00	107400.0
174.90	8197.0

Instrument :
MSVOA_V
ClientSampleId :
BFB74

176.00

177.00

177.90

104520.0

6836.0

164.0

Instrument :

MSVOA_V

ClientSampleId :

BFB74

m/z	Abundance
36.00	1505.0
37.00	9006.0
38.00	8082.0
39.00	3489.0
39.90	271.0
40.70	122.0
44.00	1437.0
45.00	1429.0
46.00	148.0
47.00	1904.0
47.90	1271.0
49.00	8097.0
50.00	34160.0
51.00	10242.0
51.90	519.0
53.00	227.0
54.90	392.0
56.00	3118.0
57.00	5919.0
58.20	207.0
59.90	1742.0
61.00	9031.0
62.00	8952.0
63.00	7667.0
64.00	957.0
65.10	1424.0
65.90	166.0
67.00	579.0
68.00	17376.0
69.00	18768.0
70.00	1233.0
72.00	1189.0
73.00	7806.0
74.00	31000.0
75.00	88888.0
76.00	8253.0
77.00	1017.0
78.00	660.0
78.90	7317.0
79.90	1934.0
80.90	7415.0
81.90	1921.0
83.00	223.0
86.10	309.0
87.00	5830.0
87.90	5675.0
90.80	890.0
91.90	5033.0
93.00	8083.0
94.00	19936.0
95.00	157312.0
96.00	10963.0
97.00	237.0
103.90	1007.0
104.80	272.0
105.90	924.0
106.70	152.0
109.90	131.0
110.80	222.0
111.70	218.0
112.80	282.0
114.80	231.0
115.90	581.0
116.90	1307.0
117.80	633.0
118.90	1107.0
123.80	140.0
128.00	452.0
128.80	317.0
129.90	823.0
130.90	176.0
134.70	436.0
136.90	321.0
139.90	198.0
141.00	2020.0
141.80	263.0
143.00	2735.0
144.10	145.0
144.90	543.0
145.90	267.0
146.80	147.0
147.90	533.0
149.90	183.0
153.60	159.0
155.00	412.0
156.00	119.0
157.00	190.0
158.80	241.0
160.80	175.0
170.40	103.0
171.00	257.0
172.00	1674.0

Instrument :
MSVOA_V
ClientSampleId :
BFB74

173.00	1526.0
174.00	112104.0
175.00	8426.0
176.00	108672.0
177.00	6960.0
177.90	170.0

Instrument :
MSVOA_V
ClientSampleId :
BFB74

m/z	Abundance
36.00	1467.0
37.00	8261.0
38.00	7277.0
39.00	3118.0
40.00	287.0
40.70	100.0
43.90	1375.0
45.00	1415.0
45.90	150.0
46.90	1698.0
47.90	1171.0
49.00	7052.0
50.00	30368.0
51.00	9428.0
51.90	389.0
52.90	259.0
54.80	355.0
56.00	2963.0
57.00	5489.0
57.90	212.0
59.90	1540.0
61.00	8107.0
62.00	7993.0
63.00	7040.0
63.90	871.0
65.00	1438.0
65.90	200.0
67.00	550.0
68.00	15999.0
69.00	16888.0
70.00	1039.0
71.90	1031.0
73.00	7003.0
74.00	28424.0
75.00	81672.0
76.00	7137.0
77.00	1012.0
78.00	601.0
78.90	6544.0
79.90	1843.0
80.90	6713.0
81.90	1793.0
83.00	139.0
86.10	221.0
87.00	5499.0
87.90	4801.0
90.80	878.0
92.00	4977.0
93.00	7244.0
94.00	18016.0
95.00	141824.0
96.00	9906.0
97.10	184.0
103.90	959.0
104.70	262.0
105.90	776.0
106.70	139.0
109.80	113.0
110.80	177.0
111.70	201.0
112.80	191.0
114.80	192.0
115.80	567.0
116.90	1176.0
117.90	672.0
118.90	1013.0
123.70	106.0
127.90	411.0
128.80	363.0
129.90	693.0
130.90	225.0
134.90	429.0
136.90	318.0
139.90	175.0
141.00	1884.0
141.70	191.0
143.00	2321.0
143.90	182.0
145.00	493.0
145.80	231.0
146.70	142.0
147.90	425.0
149.90	133.0
153.60	163.0
155.00	371.0
156.00	117.0
157.00	235.0
158.70	160.0
160.80	179.0
171.00	262.0
172.00	1615.0
173.00	1557.0

Instrument :
MSVOA_V
ClientSampleId :
BFB74

174.00	106824.0
175.00	7839.0
176.00	101816.0
177.00	6450.0
177.90	165.0

Instrument :
MSVOA_V
ClientSampleId :
BFB74