

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV050919\
 Data File : VV010774.D
 Acq On : 09 May 2019 18:30
 Operator : SY/MD
 Sample : K2693-19
 Misc : 5.89G/10ML/MSVOA V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFHF4

Quant Time: May 10 06:52:52 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM050719S.M
 Quant Title : VOC Analysis
 QLast Update : Fri May 10 05:43:08 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	59330	25.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	54916	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	17791	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	19046	20.66	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.64%
7) Chloroethane-d5	1.57	69	18727	24.69	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	98.76%
10) 1,1-Dichloroethene-d2	2.13	63	32129	16.07	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	64.28%
20) 2-Butanone-d5	3.94	46	14080	50.91	ug/L	0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	101.82%
24) Chloroform-d	4.40	84	38761	23.96	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	95.84%
26) 1,2-Dichloroethane-d4	5.08	65	26292	26.03	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	104.12%
29) Benzene-d6	5.10	84	74824	25.89	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	103.56%
33) 1,2-Dichloropropane-d6	6.12	67	24818	26.95	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	107.80%
37) Toluene-d8	7.36	98	60902	22.00	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	88.00%
38) trans-1,3-Dichloropropene-	7.66	79	9521	22.68	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	90.72%
39) 2-Hexanone-d5	8.13	63	9360	48.56	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.12%
48) 1,1,2,2-Tetrachloroethane-	10.26	84	21218	24.51	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	98.04%
61) 1,2-Dichlorobenzene-d4	11.67	152	17476	25.36	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	101.44%


Target Compounds					Ovalue
13) Acetone	2.19	43	5338	12.467 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV050919\
Data File : VV010774.D
Acq On : 09 May 2019 18:30
Operator : SY/MD
Sample : K2693-19
Misc : 5.89G/10ML/MSVOA V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFHF4

Quant Time: May 10 06:52:52 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM050719S.M
Quant Title : VOC Analysis
QLast Update : Fri May 10 05:43:08 2019
Response via : Initial Calibration

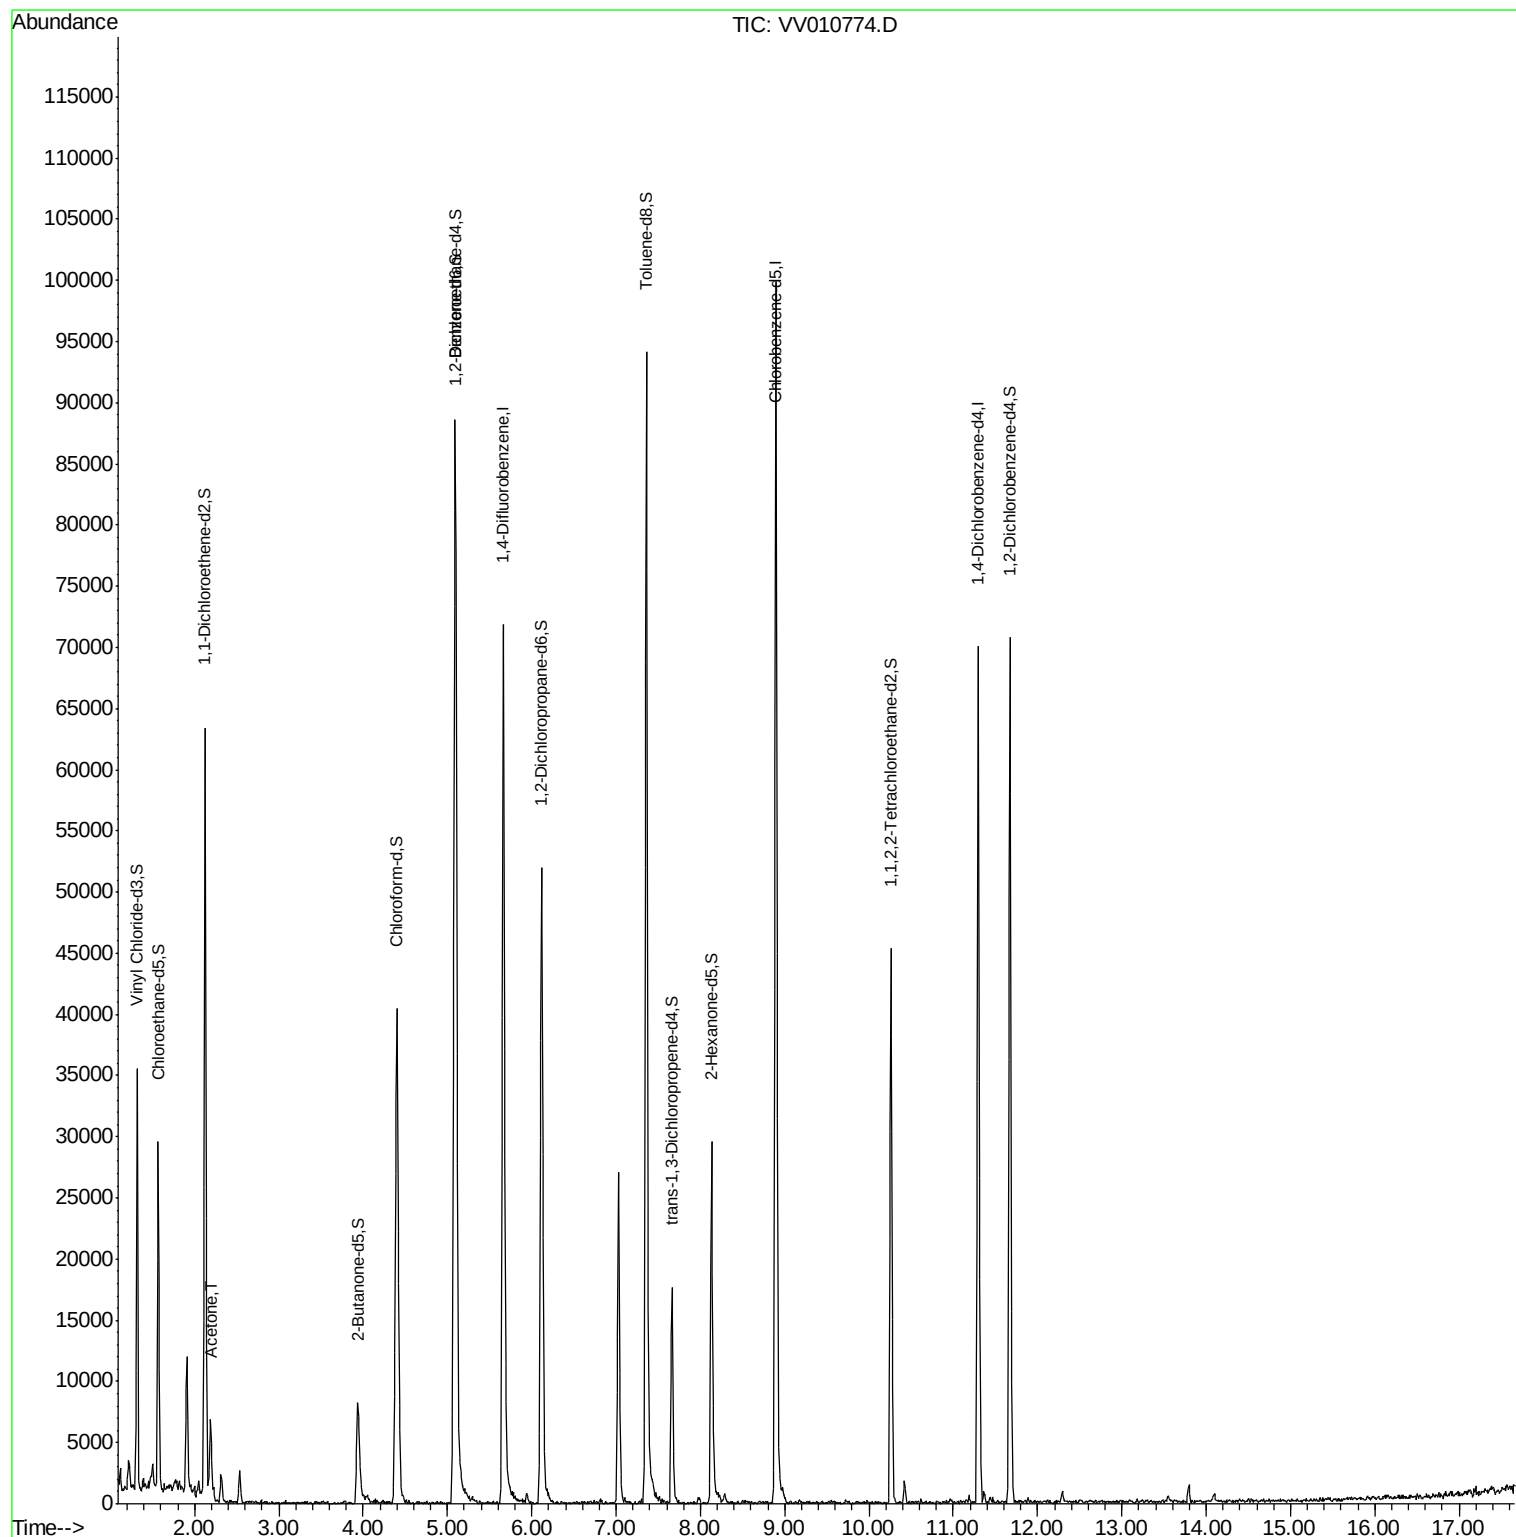

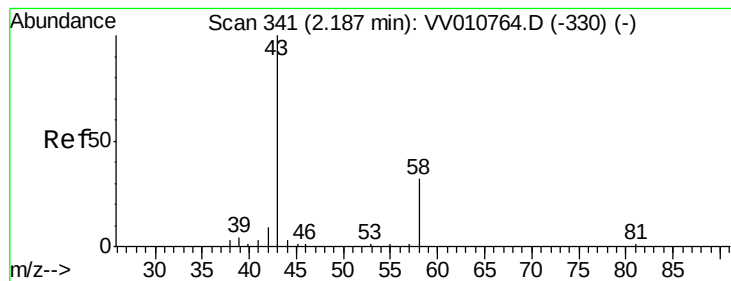

#13
 Acetone
 Concen: 12.467 ug/L
 RT: 2.19 min Scan# 342
 Delta R.T. 0.00 min
 Lab File: VV010774.D
 Acq: 09 May 2019 18:30

Instrument :
 MSVOA_V
 ClientSampleId :
 BFHF4

Tot Ion: 43 Resp: 5338
 Ion Ratio Lower Upper
 43 100
 58 31.2 0.0 63.4

