

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV050919\
 Data File : VV010784.D
 Acq On : 10 May 2019 00:03
 Operator : SY/MD
 Sample : K2690-21
 Misc : 5.46G/10ML/MSVOA V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A5167

Quant Time: May 10 08:08:18 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM050719S.M
 Quant Title : VOC Analysis
 QLast Update : Fri May 10 07:54:34 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	96509	25.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	97208	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	40185	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	24873	16.59	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	66.36%
7) Chloroethane-d5	1.58	69	25416	20.60	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.40%
10) 1,1-Dichloroethene-d2	2.13	63	44263	13.61	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	54.44%
20) 2-Butanone-d5	3.94	46	20750	46.12	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	92.24%
24) Chloroform-d	4.40	84	61404	23.34	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.36%
26) 1,2-Dichloroethane-d4	5.08	65	39141	23.82	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	95.28%
29) Benzene-d6	5.10	84	110940	21.68	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	86.72%
33) 1,2-Dichloropropane-d6	6.12	67	38202	23.43	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	93.72%
37) Toluene-d8	7.36	98	102079	20.83	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	83.32%
38) trans-1,3-Dichloropropene-	7.66	79	14535	19.56	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	78.24%
39) 2-Hexanone-d5	8.13	63	15626	45.80	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	91.60%
48) 1,1,2,2-Tetrachloroethane-	10.26	84	35500	23.17	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	92.68%
61) 1,2-Dichlorobenzene-d4	11.67	152	38367	24.65	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	98.60%


Target Compounds					Ovalue
13) Acetone	2.19	43	3575	5.133 ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV050919\
Data File : VV010784.D
Acq On : 10 May 2019 00:03
Operator : SY/MD
Sample : K2690-21
Misc : 5.46G/10ML/MSVOA V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A5167

Quant Time: May 10 08:08:18 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM050719S.M
Quant Title : VOC Analysis
QLast Update : Fri May 10 07:54:34 2019
Response via : Initial Calibration

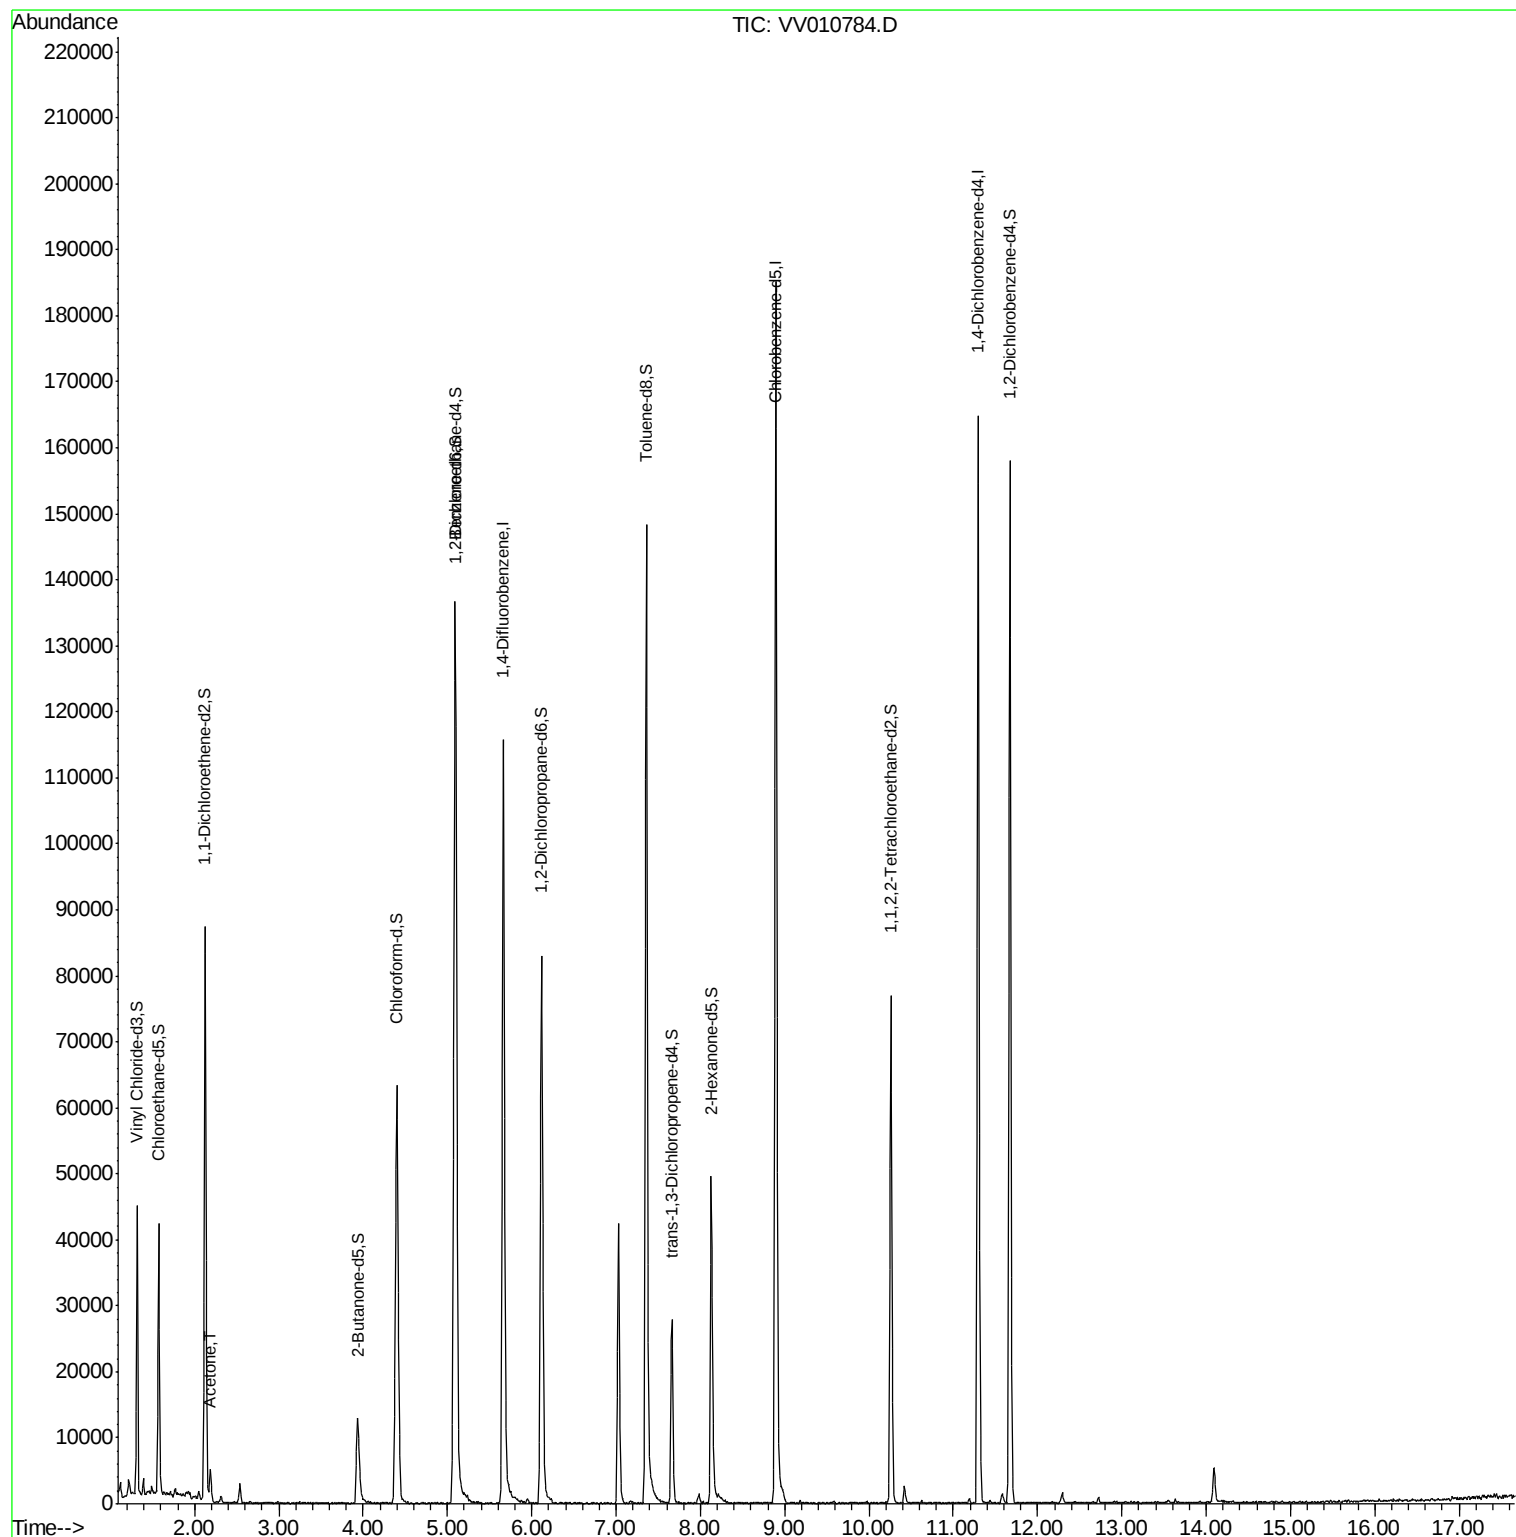

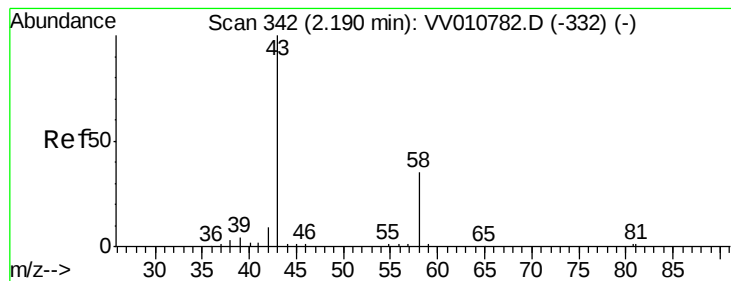

#13
 Acetone
 Concen: 5.133 ug/L
 RT: 2.19 min Scan# 342
 Delta R.T. -0.00 min
 Lab File: VV010784.D
 Acq: 10 May 2019 00:03

Instrument :
 MSVOA_V
 ClientSampleId :
 A5167

Tot Ion: 43 Resp: 3575
 Ion Ratio Lower Upper
 43 100
 58 28.1 0.0 63.4

