

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV050919\
 Data File : VV010797.D
 Acq On : 10 May 2019 06:04
 Operator : SY/MD
 Sample : K2788-01
 Misc : 7.11G/10ML/MSVOA V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A5188

Quant Time: May 10 09:06:49 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM050719S.M
 Quant Title : VOC Analysis
 QLast Update : Fri May 10 07:54:34 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	101811	25.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	100389	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	38175	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	26541	16.78	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	67.12%
7) Chloroethane-d5	1.56	69	26994	20.74	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.96%
10) 1,1-Dichloroethene-d2	2.12	63	34470	10.05	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	40.20%#
20) 2-Butanone-d5	3.92	46	23187	48.86	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.72%
24) Chloroform-d	4.39	84	61319	22.09	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	88.36%
26) 1,2-Dichloroethane-d4	5.07	65	41456	23.91	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	95.64%
29) Benzene-d6	5.09	84	119973	22.71	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	90.84%
33) 1,2-Dichloropropane-d6	6.11	67	39981	23.75	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	95.00%
37) Toluene-d8	7.36	98	105772	20.90	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	83.60%
38) trans-1,3-Dichloropropene-	7.66	79	15489	20.18	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	80.72%
39) 2-Hexanone-d5	8.13	63	17606	49.97	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	99.94%
48) 1,1,2,2-Tetrachloroethane-	10.26	84	39639	25.05	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	100.20%
61) 1,2-Dichlorobenzene-d4	11.67	152	35622	24.09	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	96.36%


Target Compounds					Ovalue
13) Acetone	2.18	43	2812	3.827 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV050919\
Data File : VV010797.D
Acq On : 10 May 2019 06:04
Operator : SY/MD
Sample : K2788-01
Misc : 7.11G/10ML/MSVOA V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A5188

Quant Time: May 10 09:06:49 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM050719S.M
Quant Title : VOC Analysis
QLast Update : Fri May 10 07:54:34 2019
Response via : Initial Calibration

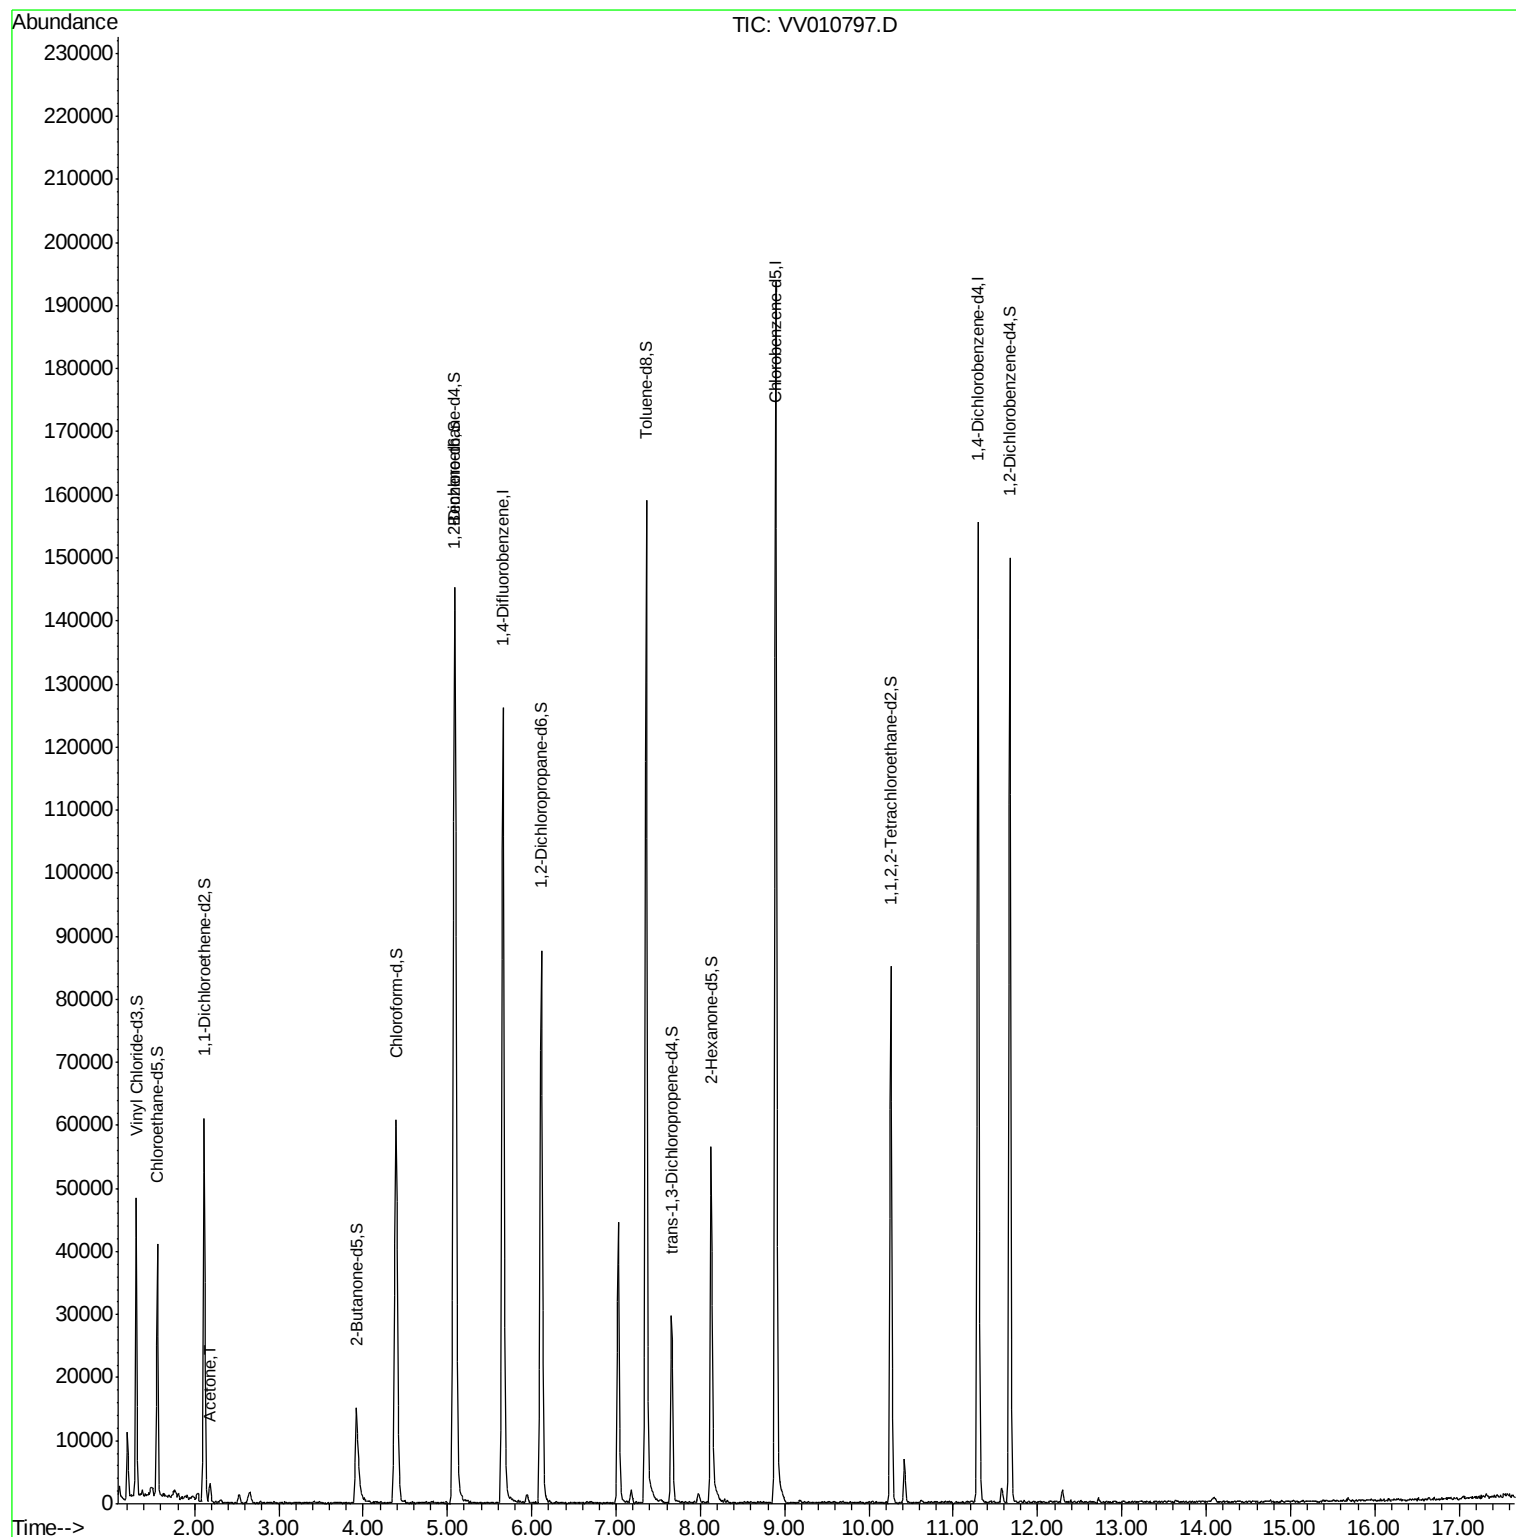

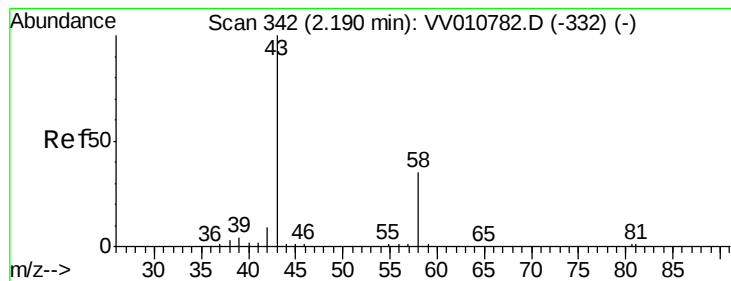

#13
 Acetone
 Concen: 3.827 ug/L
 RT: 2.18 min Scan# 340
 Delta R.T. -0.01 min
 Lab File: VV010797.D
 Acq: 10 May 2019 06:04

Instrument :
 MSVOA_V
 ClientSampleId :
 A5188

Tot Ion: 43 Resp: 2812
 Ion Ratio Lower Upper
 43 100
 58 30.6 0.0 63.4

