


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050919\
 Data File : VV010763.D
 Acq On : 09 May 2019 11:25
 Operator : SY/MD
 Sample : BFB96
 Misc : 5.00G/10ML/MSVOA_V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB96

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM050719S.M
 Title : VOC Analysis
 Last Update : Thu May 09 04:43:30 2019

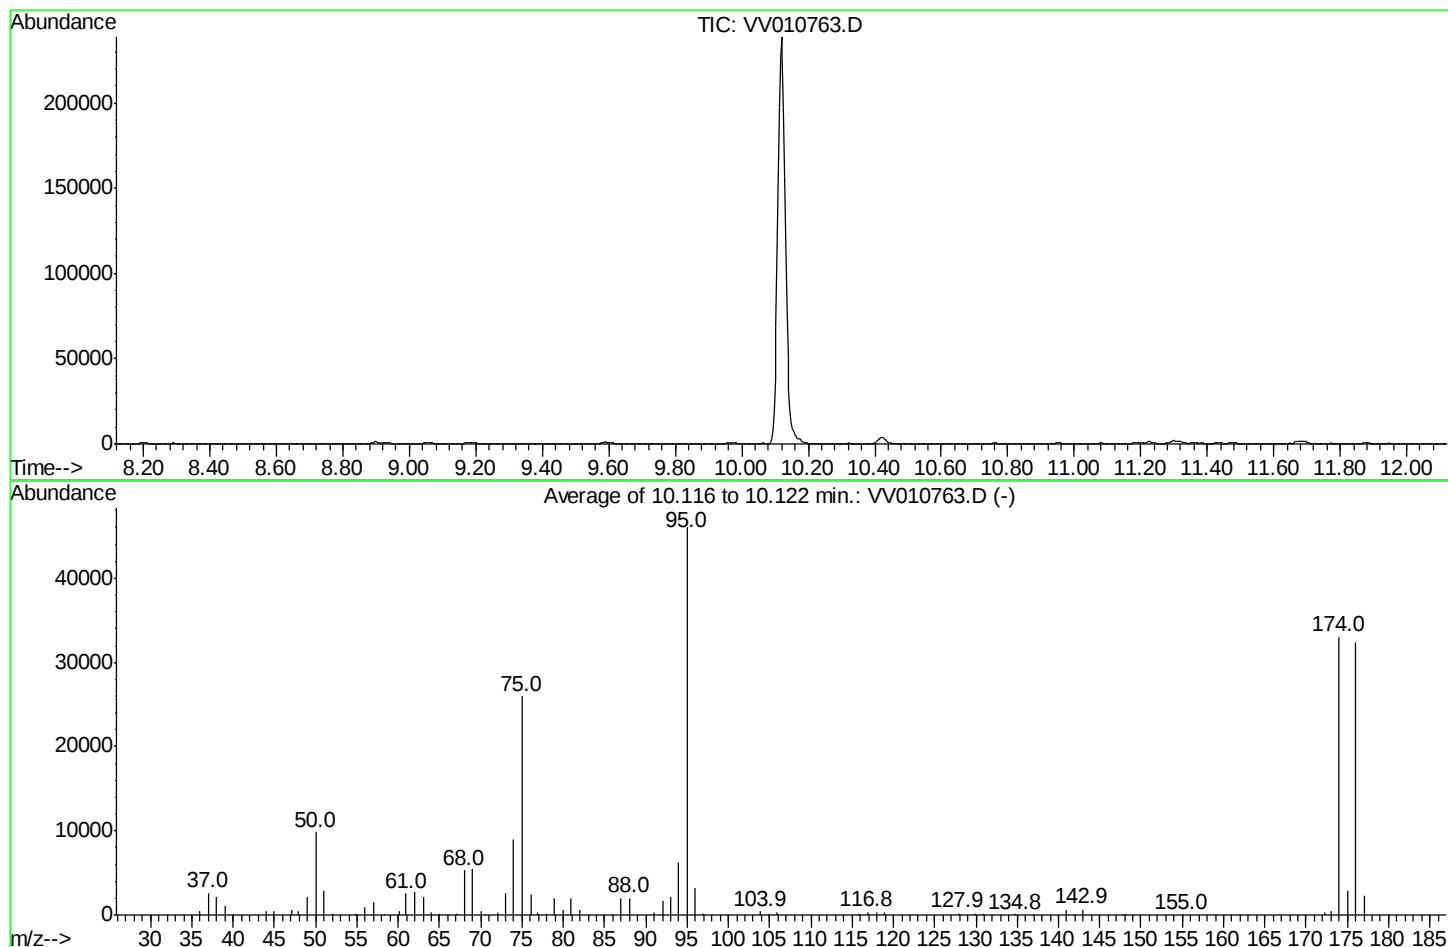

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.4	9861	PASS
75	95	30	80	56.4	25949	PASS
95	95	100	100	100.0	46048	PASS
96	95	5	9	7.0	3234	PASS
173	174	0.00	2	1.3	425	PASS
174	95	50	120	71.8	33040	PASS
175	174	5	9	8.6	2834	PASS
176	174	95	101	97.9	32362	PASS
177	176	5	9	7.0	2256	PASS

m/z	Abundance
40.00	112.0
44.00	179.0

Instrument :
MSVOA_V
ClientSampleId :
BFB96

m/z	Abundance
35.90	495.0
37.00	2554.0
38.00	2102.0
39.00	1096.0
39.90	195.0
44.00	587.0
45.00	471.0
47.00	526.0
47.90	399.0
49.00	2180.0
50.00	9901.0
51.00	3101.0
52.00	192.0
54.90	174.0
56.00	938.0
57.10	1479.0
58.20	109.0
60.10	484.0
60.90	2370.0
62.00	2632.0
63.00	2107.0
63.90	233.0
64.90	189.0
67.00	235.0
68.00	5395.0
69.00	5420.0
70.00	406.0
72.00	300.0
73.00	2551.0
74.00	8935.0
75.00	25824.0
76.00	2450.0
77.00	313.0
77.90	205.0
78.90	2085.0
80.00	576.0
80.90	2000.0
81.90	525.0
87.00	2046.0
88.00	1991.0
91.00	352.0
92.00	1602.0
93.00	2135.0
94.00	6262.0
95.00	45664.0
96.00	3204.0
96.90	125.0
103.90	340.0
104.90	112.0
106.00	358.0
115.80	163.0
116.80	345.0
118.00	240.0
118.90	250.0
127.90	204.0
129.90	194.0
130.80	103.0
134.80	135.0
141.00	611.0
141.80	102.0
142.90	653.0
147.80	105.0
148.00	108.0
172.30	289.0
174.00	32488.0
175.00	2718.0
176.00	30640.0
177.00	2304.0

Instrument :
MSVOA_V
ClientSampleId :
BFB96

m/z	Abundance
35.90	494.0
37.00	2695.0
38.00	2268.0
39.00	1041.0
39.90	186.0
44.00	591.0
45.00	532.0
47.10	552.0
47.90	465.0
49.00	2230.0
50.00	10158.0
51.00	2984.0
52.00	170.0
54.90	230.0
56.00	948.0
57.00	1594.0
60.00	491.0
60.90	2612.0
62.00	2931.0
63.00	2297.0
64.00	250.0
65.00	184.0
67.10	241.0
68.00	5442.0
69.00	5717.0
70.00	430.0
72.00	339.0
73.00	2617.0
74.00	9374.0
75.00	26712.0
76.00	2483.0
76.80	280.0
77.90	210.0
78.90	2018.0
80.00	618.0
80.90	2106.0
81.90	569.0
87.00	1970.0
88.00	2095.0
90.90	347.0
92.00	1698.0
93.00	2215.0
94.00	6514.0
95.00	47352.0
96.00	3363.0
97.00	154.0
103.90	405.0
104.90	109.0
106.00	294.0
115.90	187.0
116.90	360.0
117.90	262.0
118.90	279.0
127.90	224.0
129.90	189.0
130.80	120.0
134.80	120.0
136.90	103.0
140.90	668.0
142.90	722.0
147.70	111.0
148.00	105.0
172.20	299.0
173.00	661.0
174.00	33960.0
175.00	2938.0
176.00	33472.0
177.00	2341.0

Instrument :
MSVOA_V
ClientSampleId :
BFB96

m/z	Abundance
35.90	458.0
37.00	2677.0
38.00	2164.0
39.00	924.0
39.90	170.0
44.00	565.0
45.00	567.0
47.10	542.0
47.90	448.0
49.00	2077.0
50.00	9524.0
51.00	2739.0
52.10	175.0
54.90	254.0
56.00	890.0
57.00	1579.0
60.00	463.0
61.00	2593.0
62.00	2858.0
63.00	2171.0
64.10	272.0
65.00	191.0
67.10	199.0
68.00	4962.0
69.00	5345.0
70.00	395.0
72.10	317.0
73.00	2470.0
74.00	8821.0
75.00	25312.0
76.10	2192.0
76.80	243.0
77.90	176.0
78.90	1869.0
79.90	576.0
80.90	2015.0
82.00	551.0
85.90	116.0
87.00	1738.0
88.00	1865.0
90.90	287.0
92.00	1620.0
93.00	2062.0
94.00	6040.0
95.00	45128.0
96.00	3135.0
97.00	146.0
103.90	432.0
104.90	104.0
105.80	240.0
115.90	187.0
116.90	364.0
117.90	251.0
118.90	332.0
127.90	204.0
129.80	202.0
130.80	102.0
136.80	103.0
140.90	712.0
142.90	687.0
155.00	100.0
172.20	264.0
173.00	614.0
174.00	32672.0
175.00	2848.0
176.00	32976.0
177.00	2123.0

Instrument :
MSVOA_V
ClientSampleId :
BFB96