
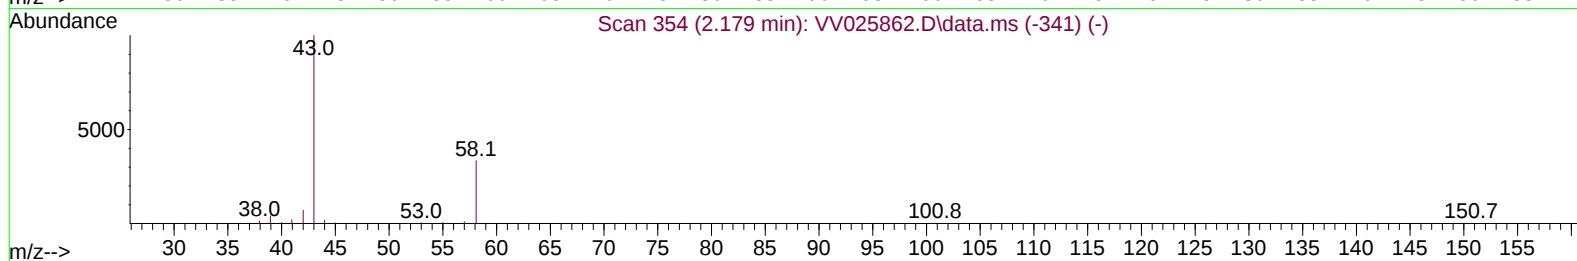
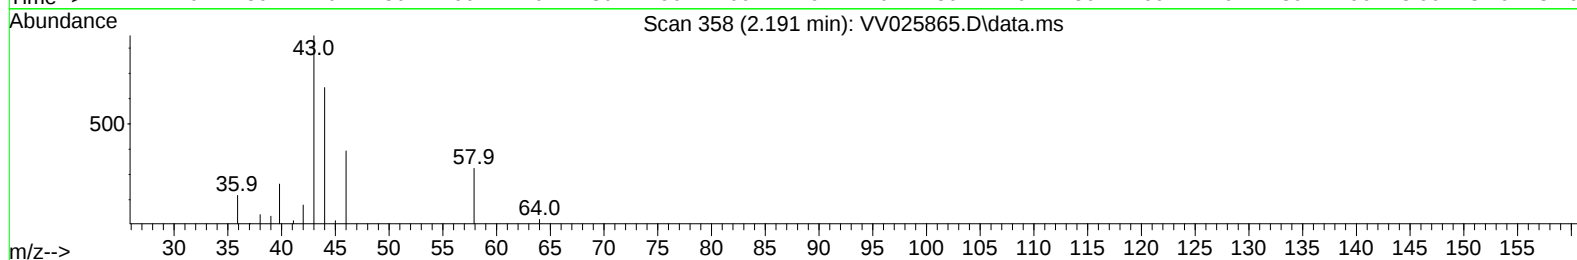


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051022\
 Data File : VV025865.D
 Acq On : 10 May 2022 17:09
 Operator : SY/MD
 Sample : N2713-03
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Quant Time: May 11 04:25:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed May 11 04:11:56 2022
 Response via : Initial Calibration

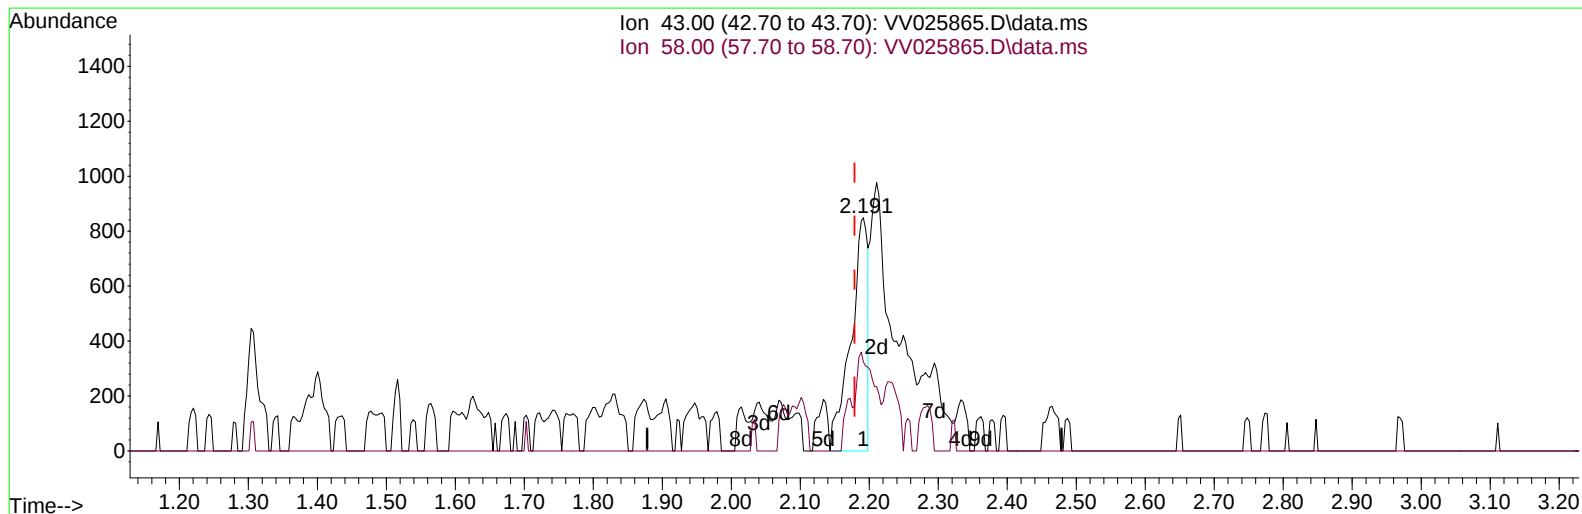

TIC: VV025865.D\data.ms

(13) Acetone (T)

2.191min (+ 0.013) 4.37 ug/L

response 1437

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.50	46.28
0.00	0.00	0.00
0.00	0.00	0.00