




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051022\
 Data File : VV025865.D
 Acq On : 10 May 2022 17:09
 Operator : SY/MD
 Sample : N2713-03
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW2X9ME

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 05/18/2022
 Supervised By :Mahesh Dadoda 05/18/2022

Quant Time: May 11 04:25:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed May 11 04:11:56 2022
 Response via : Initial Calibration

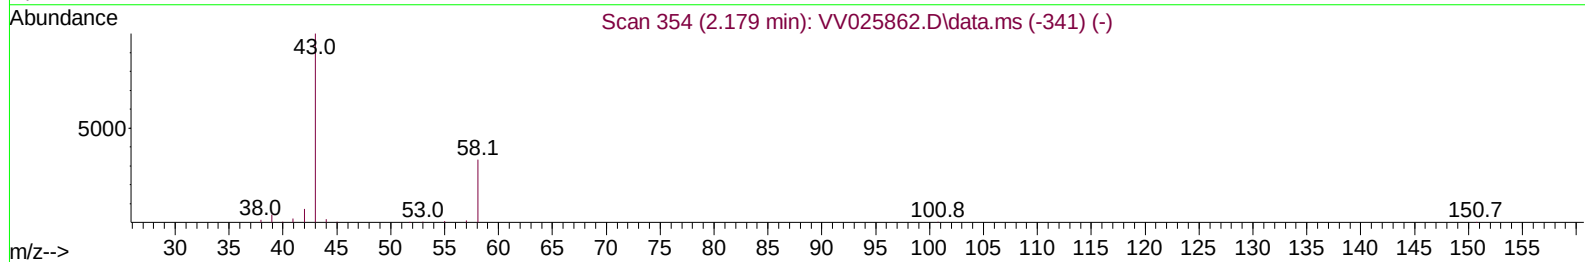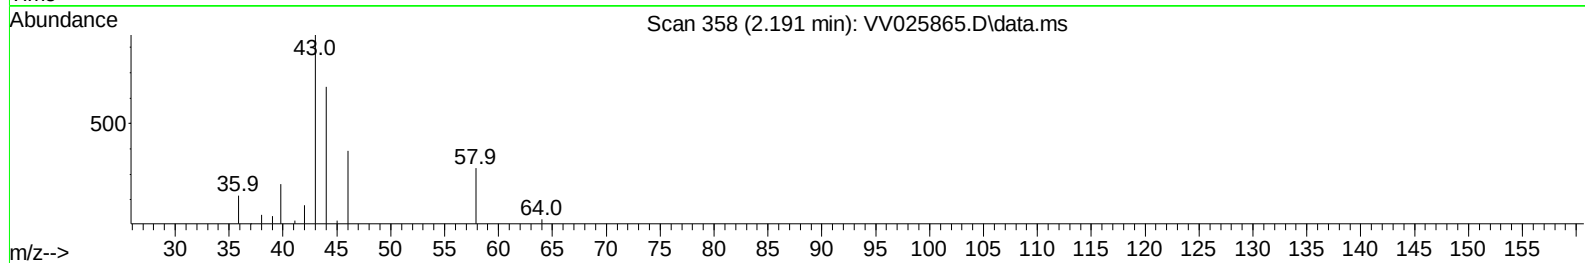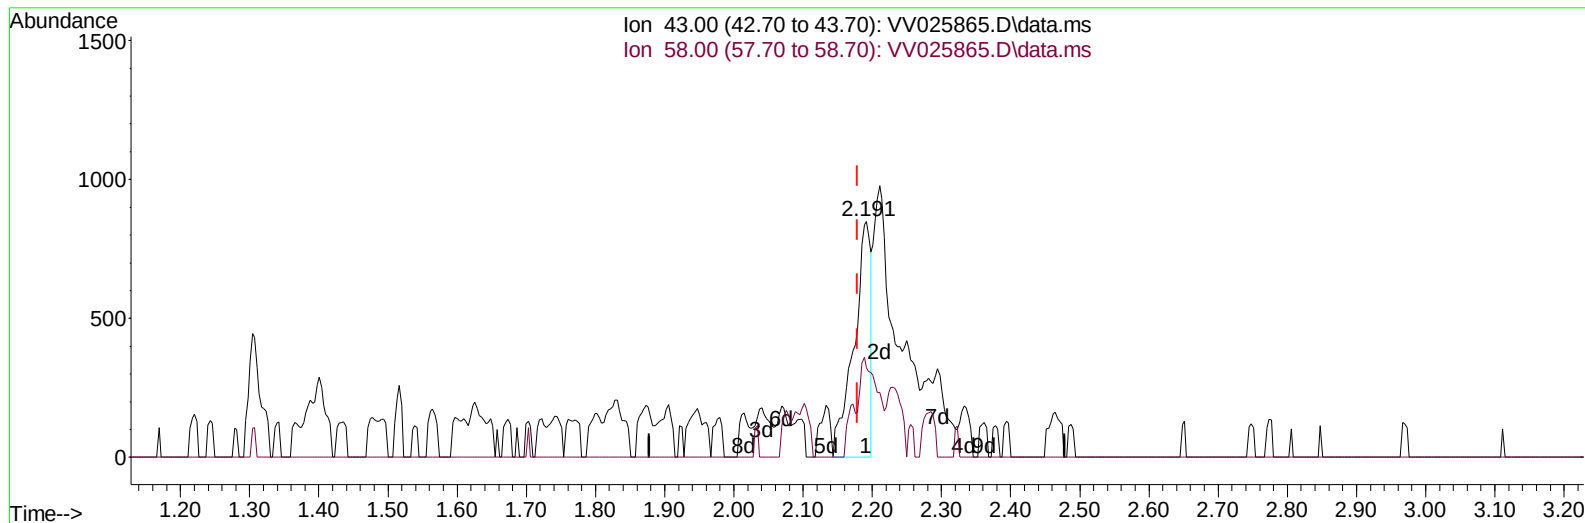

TIC: VV025865.D\data.ms

(13) Acetone (T)

2.191min (+ 0.013) 4.37 ug/L

response 1437

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.50	46.28
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051022\
 Data File : VV025865.D
 Acq On : 10 May 2022 17:09
 Operator : SY/MD
 Sample : N2713-03
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW2X9ME

Manual IntegrationsAPPROVED

Quant Time: May 11 04:25:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed May 11 04:11:56 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 05/18/2022
 Supervised By :Mahesh Dadoda 05/18/2022

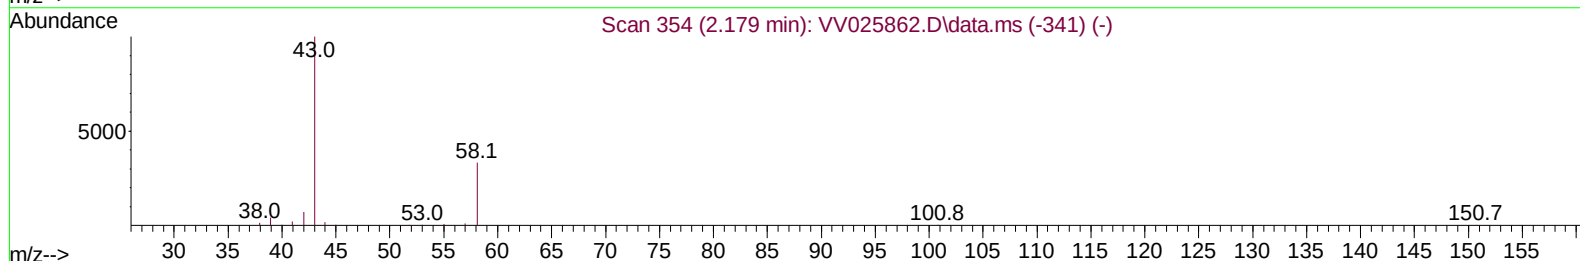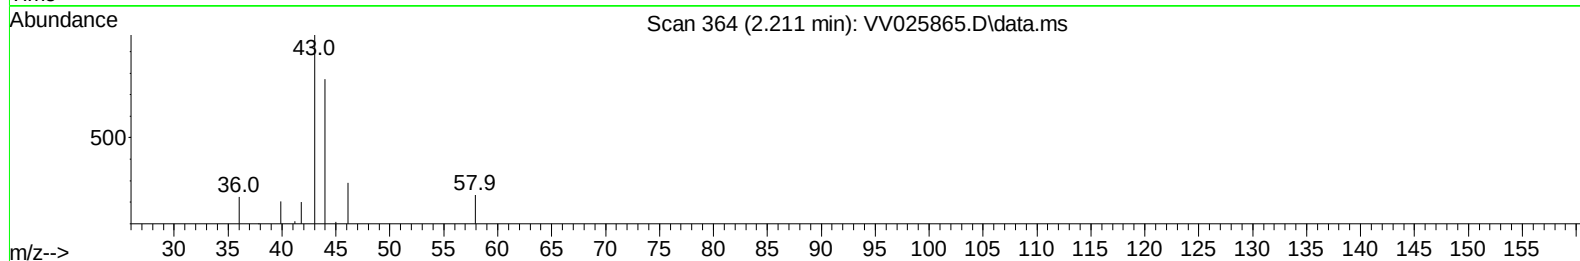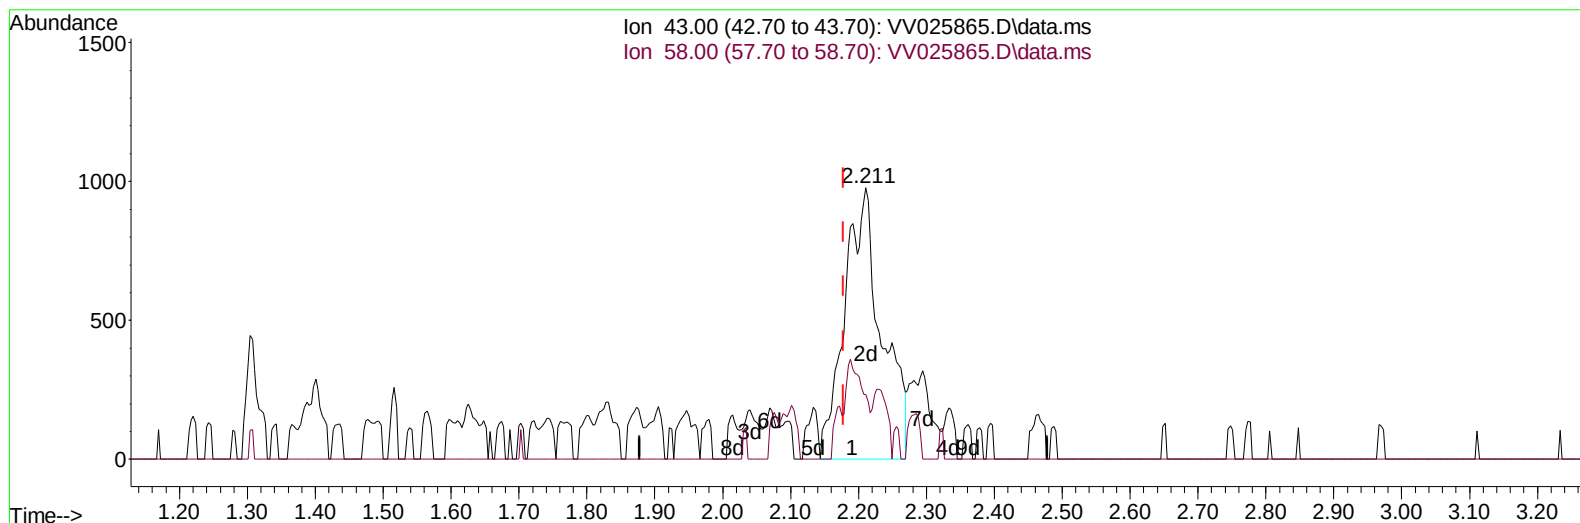

TIC: VV025865.D\data.ms

(13) Acetone (T)

2.211min (+ 0.032) 11.19 ug/L m

response 3685

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.50	18.05
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051022\
 Data File : VV025865.D
 Acq On : 10 May 2022 17:09
 Operator : SY/MD
 Sample : N2713-03
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW2X9ME

Manual IntegrationsAPPROVED

Reviewed By : John Carlone 05/18/2022
 Supervised By : Mahesh Dadoda 05/18/2022

Quant Time: May 11 04:25:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed May 11 04:11:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	87212	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	85941	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	38099	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	60202	53.487	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	106.980%	
7) Chloroethane-d5	1.568	69	48478	49.045	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	98.080%	
11) 1,1-Dichloroethene-d2	2.108	63	84685	43.019	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	86.040%	
21) 2-Butanone-d5	3.912	46	40968	84.921	ug/L	0.03
Spiked Amount 100.000	Range 40	- 130	Recovery	=	84.920%	
24) Chloroform-d	4.349	84	80602	51.270	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	102.540%	
26) 1,2-Dichloroethane-d4	5.034	65	53059	55.844	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	111.680%	
32) Benzene-d6	5.050	84	167213	55.811	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	111.620%	
36) 1,2-Dichloropropane-d6	6.069	67	52176	56.701	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	113.400%	
41) Toluene-d8	7.317	98	136723	49.529	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	99.060%	
43) trans-1,3-Dichloroprop...	7.625	79	20112	48.962	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	97.920%	
47) 2-Hexanone-d5	8.092	63	30247	89.656	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	89.660%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	64304	52.401	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	104.800%	
66) 1,2-Dichlorobenzene-d4	11.622	152	47755	57.142	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	114.280%	
Target Compounds						
13) Acetone	2.211	43	3685m	11.194	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051022\
Data File : VV025865.D
Acq On : 10 May 2022 17:09
Operator : SY/MD
Sample : N2713-03
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW2X9ME

Manual IntegrationsAPPROVED

Quant Time: May 11 04:25:07 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis
QLast Update : Wed May 11 04:11:56 2022
Response via : Initial Calibration

Reviewed By :John Carlone 05/18/2022
Supervised By :Mahesh Dadoda 05/18/2022

