




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051022\
 Data File : VV025866.D
 Acq On : 10 May 2022 17:32
 Operator : SY/MD
 Sample : N2713-11
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBSK9

Manual IntegrationsAPPROVED

Quant Time: May 11 04:25:21 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed May 11 04:11:56 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 05/18/2022
 Supervised By :Mahesh Dadoda 05/18/2022

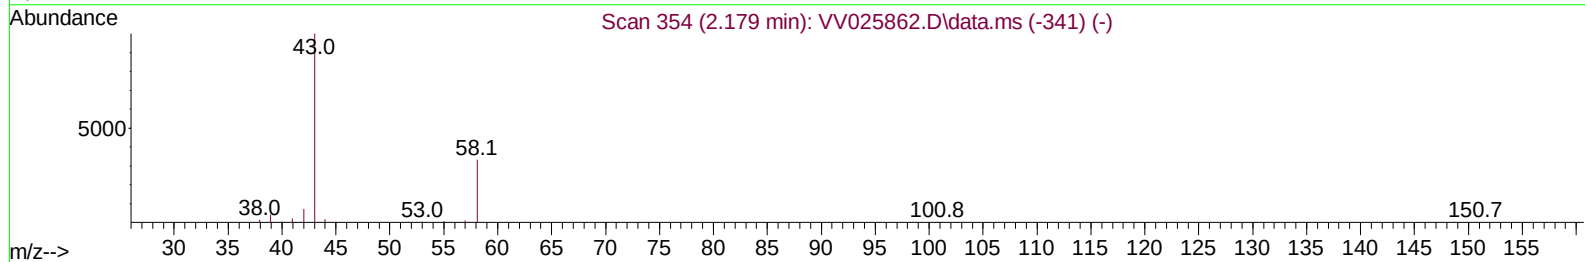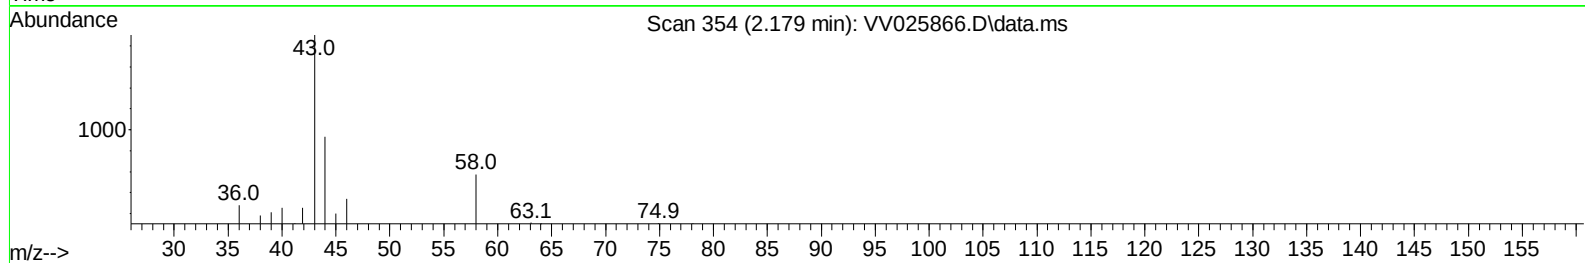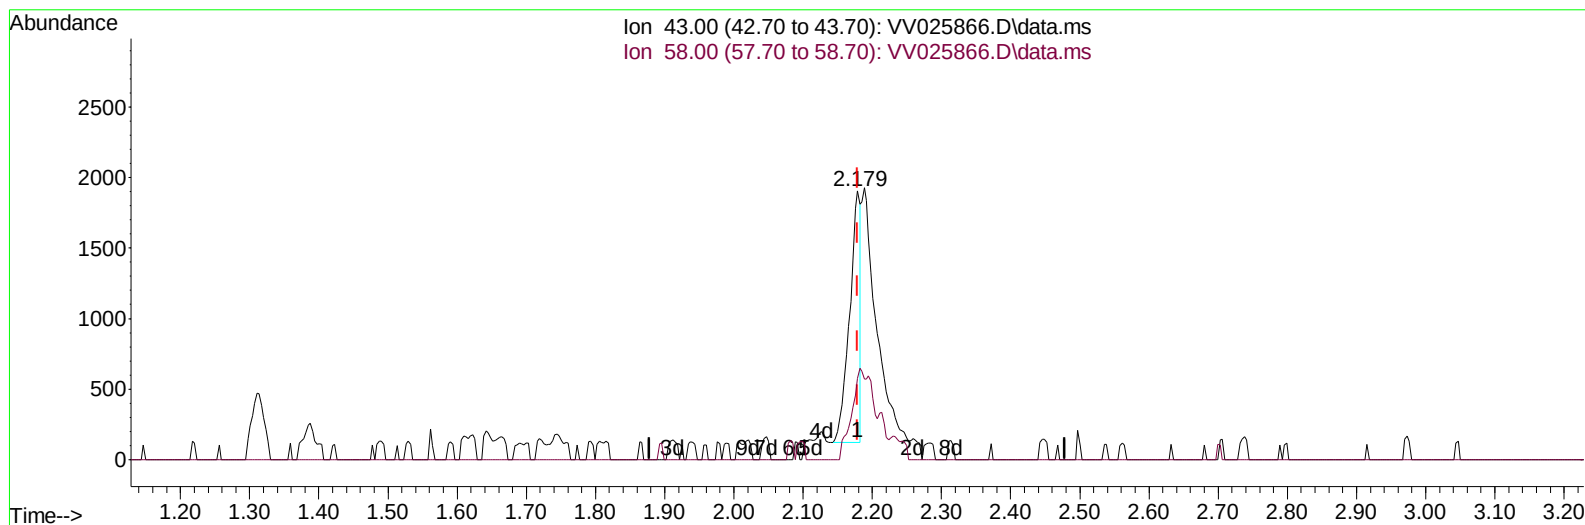

TIC: VV025866.D\data.ms

(13) Acetone (T)

2.179min (+ 0.000) 3.59 ug/L

response 1895

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.50	48.87
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051022\
Data File : VV025866.D
Acq On : 10 May 2022 17:32
Operator : SY/MD
Sample : N2713-11
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBSK9

Manual IntegrationsAPPROVED

Quant Time: May 11 04:25:21 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis
QLast Update : Wed May 11 04:11:56 2022
Response via : Initial Calibration

Reviewed By :John Carlone 05/18/2022
Supervised By :Mahesh Dadoda 05/18/2022

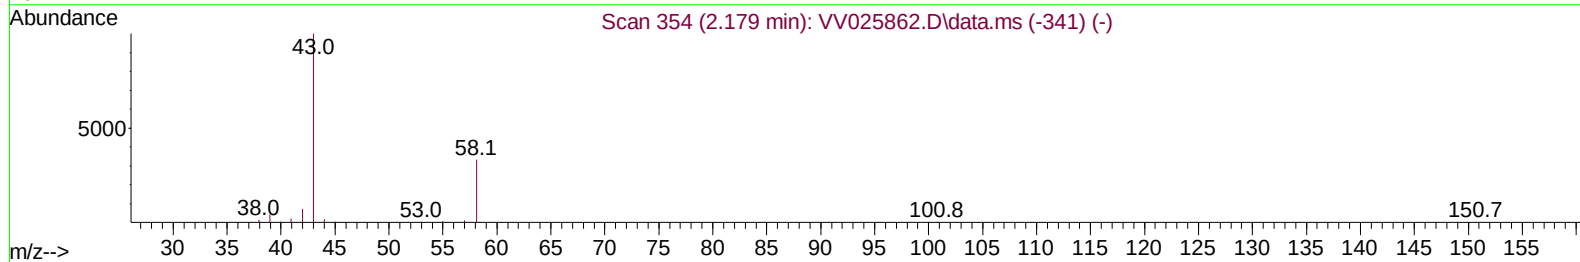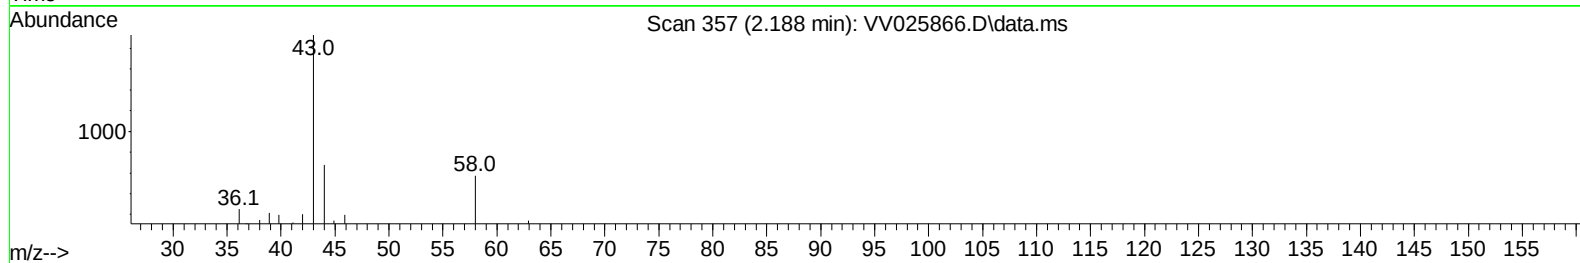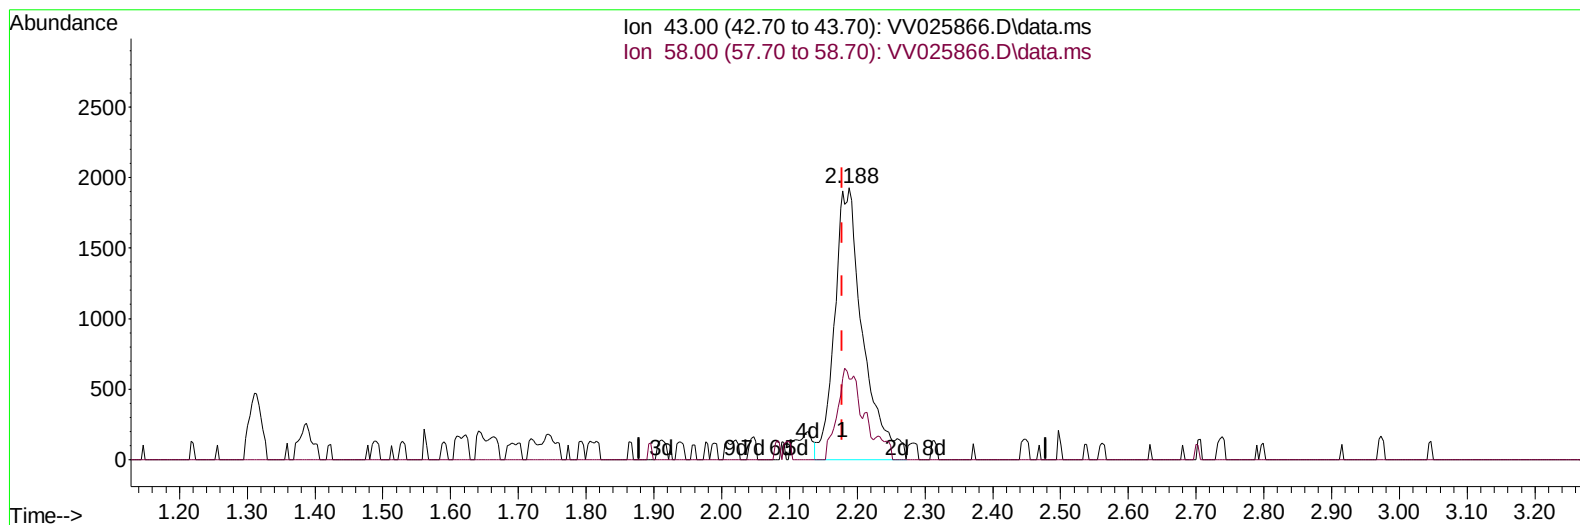

TIC: VV025866.D\data.ms

(13) Acetone (T)

2.188min (+ 0.010) 10.55 ug/L m

response 5570

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.50	16.62
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051022\
 Data File : VV025866.D
 Acq On : 10 May 2022 17:32
 Operator : SY/MD
 Sample : N2713-11
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBSK9

Manual IntegrationsAPPROVED

Quant Time: May 11 04:25:21 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed May 11 04:11:56 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 05/18/2022
 Supervised By :Mahesh Dadoda 05/18/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.619	114		139860	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117		139919	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152		60471	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.307	65		87670	48.570	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135		Recovery	=	97.140%	
7) Chloroethane-d5	1.571	69		75874	47.866	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130		Recovery	=	95.740%	
11) 1,1-Dichloroethene-d2	2.108	63		121807	38.584	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125		Recovery	=	77.160%	
21) 2-Butanone-d5	3.899	46		71891	92.924	ug/L	0.02
Spiked Amount 100.000	Range 40	- 130		Recovery	=	92.920%	
24) Chloroform-d	4.352	84		122426	48.560	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	97.120%	
26) 1,2-Dichloroethane-d4	5.034	65		79337	52.069	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	104.140%	
32) Benzene-d6	5.050	84		253915	52.055	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	104.120%	
36) 1,2-Dichloropropane-d6	6.069	67		79311	52.939	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120		Recovery	=	105.880%	
41) Toluene-d8	7.317	98		211010	46.951	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery	=	93.900%	
43) trans-1,3-Dichloroprop...	7.622	79		31565	47.199	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125		Recovery	=	94.400%	
47) 2-Hexanone-d5	8.088	63		45108	82.125	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130		Recovery	=	82.120%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84		93945	47.022	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120		Recovery	=	94.040%	
66) 1,2-Dichlorobenzene-d4	11.622	152		72975	55.014	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery	=	110.020%	
Target Compounds							
13) Acetone	2.188	43		5570m	10.550	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051022\
Data File : VV025866.D
Acq On : 10 May 2022 17:32
Operator : SY/MD
Sample : N2713-11
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBSK9

Manual IntegrationsAPPROVED

Quant Time: May 11 04:25:21 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis
QLast Update : Wed May 11 04:11:56 2022
Response via : Initial Calibration

Reviewed By :John Carlone 05/18/2022
Supervised By :Mahesh Dadoda 05/18/2022

