

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW051022\
 Data File : VW025865.D
 Acq On : 10 May 2022 17:09
 Operator : SY/MD
 Sample : N2714-08ME
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW2X9ME

Quant Time: May 11 04:25:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed May 11 04:11:56 2022
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 05/18/2022
 Supervised By : Mahesh Dadoda 05/18/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	87212	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	85941	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	38099	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	60202	53.487	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 106.980%			
7) Chloroethane-d5	1.568	69	48478	49.045	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 98.080%			
11) 1,1-Dichloroethene-d2	2.108	63	84685	43.019	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 86.040%			
21) 2-Butanone-d5	3.912	46	40968	84.921	ug/L	0.03
Spiked Amount 100.000	Range 40 - 130		Recovery = 84.920%			
24) Chloroform-d	4.349	84	80602	51.270	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 102.540%			
26) 1,2-Dichloroethane-d4	5.034	65	53059	55.844	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 111.680%			
32) Benzene-d6	5.050	84	167213	55.811	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 111.620%			
36) 1,2-Dichloropropane-d6	6.069	67	52176	56.701	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 113.400%			
41) Toluene-d8	7.317	98	136723	49.529	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 99.060%			
43) trans-1,3-Dichloroprop...	7.625	79	20112	48.962	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 97.920%			
47) 2-Hexanone-d5	8.092	63	30247	89.656	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 89.660%			
56) 1,1,2,2-Tetrachloroeth...	10.214	84	64304	52.401	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 104.800%			
66) 1,2-Dichlorobenzene-d4	11.622	152	47755	57.142	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 114.280%			
Target Compounds					Qvalue	
13) Acetone	2.211	43	3685m	11.194	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051022\
Data File : VV025865.D
Acq On : 10 May 2022 17:09
Operator : SY/MD
Sample : N2714-08ME
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
EW2X9ME

Manual Integrations
APPROVED

Reviewed By : John Carlone 05/18/2022
Supervised By : Mahesh Dadoda 05/18/2022


Quant Time: May 11 04:25:07 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis
QLast Update : Wed May 11 04:11:56 2022
Response via : Initial Calibration

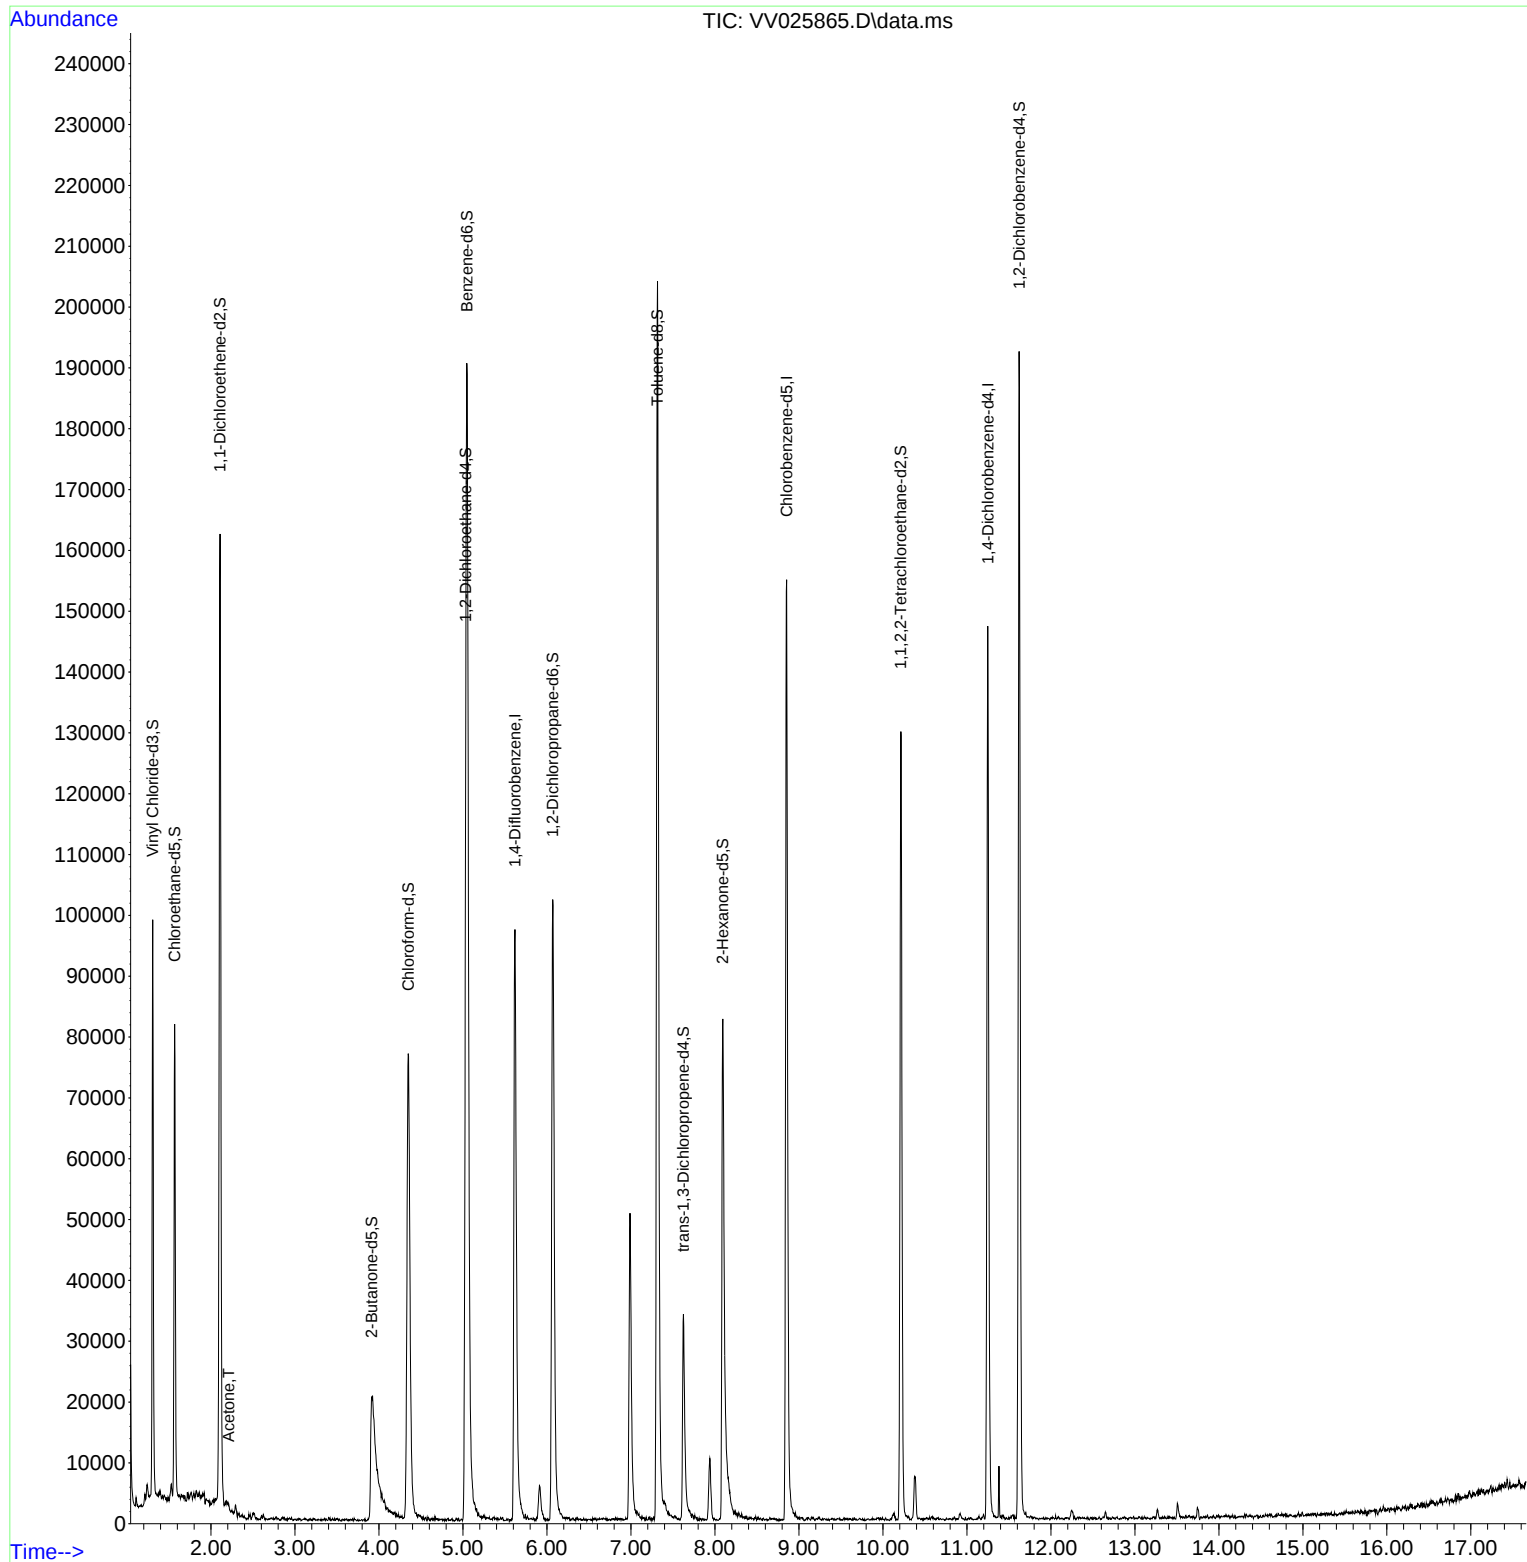

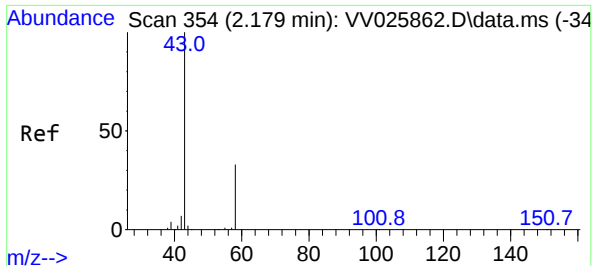

#13
Acetone
Concen: 11.194 ug/L m
RT: 2.211 min Scan# 30
Delta R.T. 0.032 min
Lab File: VV025865.D
Acq: 10 May 2022 17:09

Instrument :
MSVOA_V
ClientSampleId :
EW2X9ME

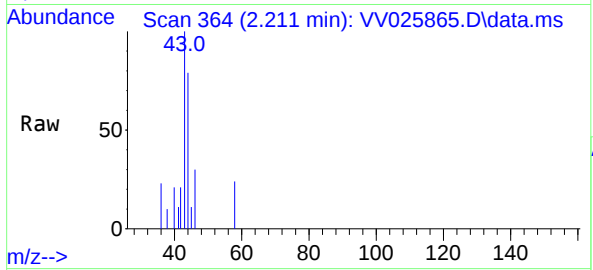

Tgt Ion: 43 Resp: 368
Ion Ratio Lower Upper
43 100
58 18.0 0.0 65.0

Manual Integrations
APPROVED

Reviewed By :John Carlone 05/18/2022
Supervised By :Mahesh Dadoda 05/18/2022

