

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051022\
 Data File : VV025866.D
 Acq On : 10 May 2022 17:32
 Operator : SY/MD
 Sample : N2713-11
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBSK9

Manual Integrations
 APPROVED

Reviewed By : John Carlone 05/18/2022
 Supervised By : Mahesh Dadoda 05/18/2022

Quant Time: May 11 04:25:21 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed May 11 04:11:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	139860	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	139919	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	60471	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	87670	48.570	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	97.140%		
7) Chloroethane-d5	1.571	69	75874	47.866	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	95.740%		
11) 1,1-Dichloroethene-d2	2.108	63	121807	38.584	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	77.160%		
21) 2-Butanone-d5	3.899	46	71891	92.924	ug/L	0.02
Spiked Amount 100.000	Range 40 - 130		Recovery =	92.920%		
24) Chloroform-d	4.352	84	122426	48.560	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	97.120%		
26) 1,2-Dichloroethane-d4	5.034	65	79337	52.069	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	104.140%		
32) Benzene-d6	5.050	84	253915	52.055	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	104.120%		
36) 1,2-Dichloropropane-d6	6.069	67	79311	52.939	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	105.880%		
41) Toluene-d8	7.317	98	211010	46.951	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	93.900%		
43) trans-1,3-Dichloroprop...	7.622	79	31565	47.199	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	94.400%		
47) 2-Hexanone-d5	8.088	63	45108	82.125	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	82.120%		
56) 1,1,2,2-Tetrachloroeth...	10.214	84	93945	47.022	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	94.040%		
66) 1,2-Dichlorobenzene-d4	11.622	152	72975	55.014	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	110.020%		
Target Compounds						Qvalue
13) Acetone	2.188	43	5570m	10.550	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051022\
Data File : VV025866.D
Acq On : 10 May 2022 17:32
Operator : SY/MD
Sample : N2713-11
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
DBSK9

Manual Integrations
APPROVED

Reviewed By : John Carlone 05/18/2022
Supervised By : Mahesh Dadoda 05/18/2022


Quant Time: May 11 04:25:21 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis
QLast Update : Wed May 11 04:11:56 2022
Response via : Initial Calibration

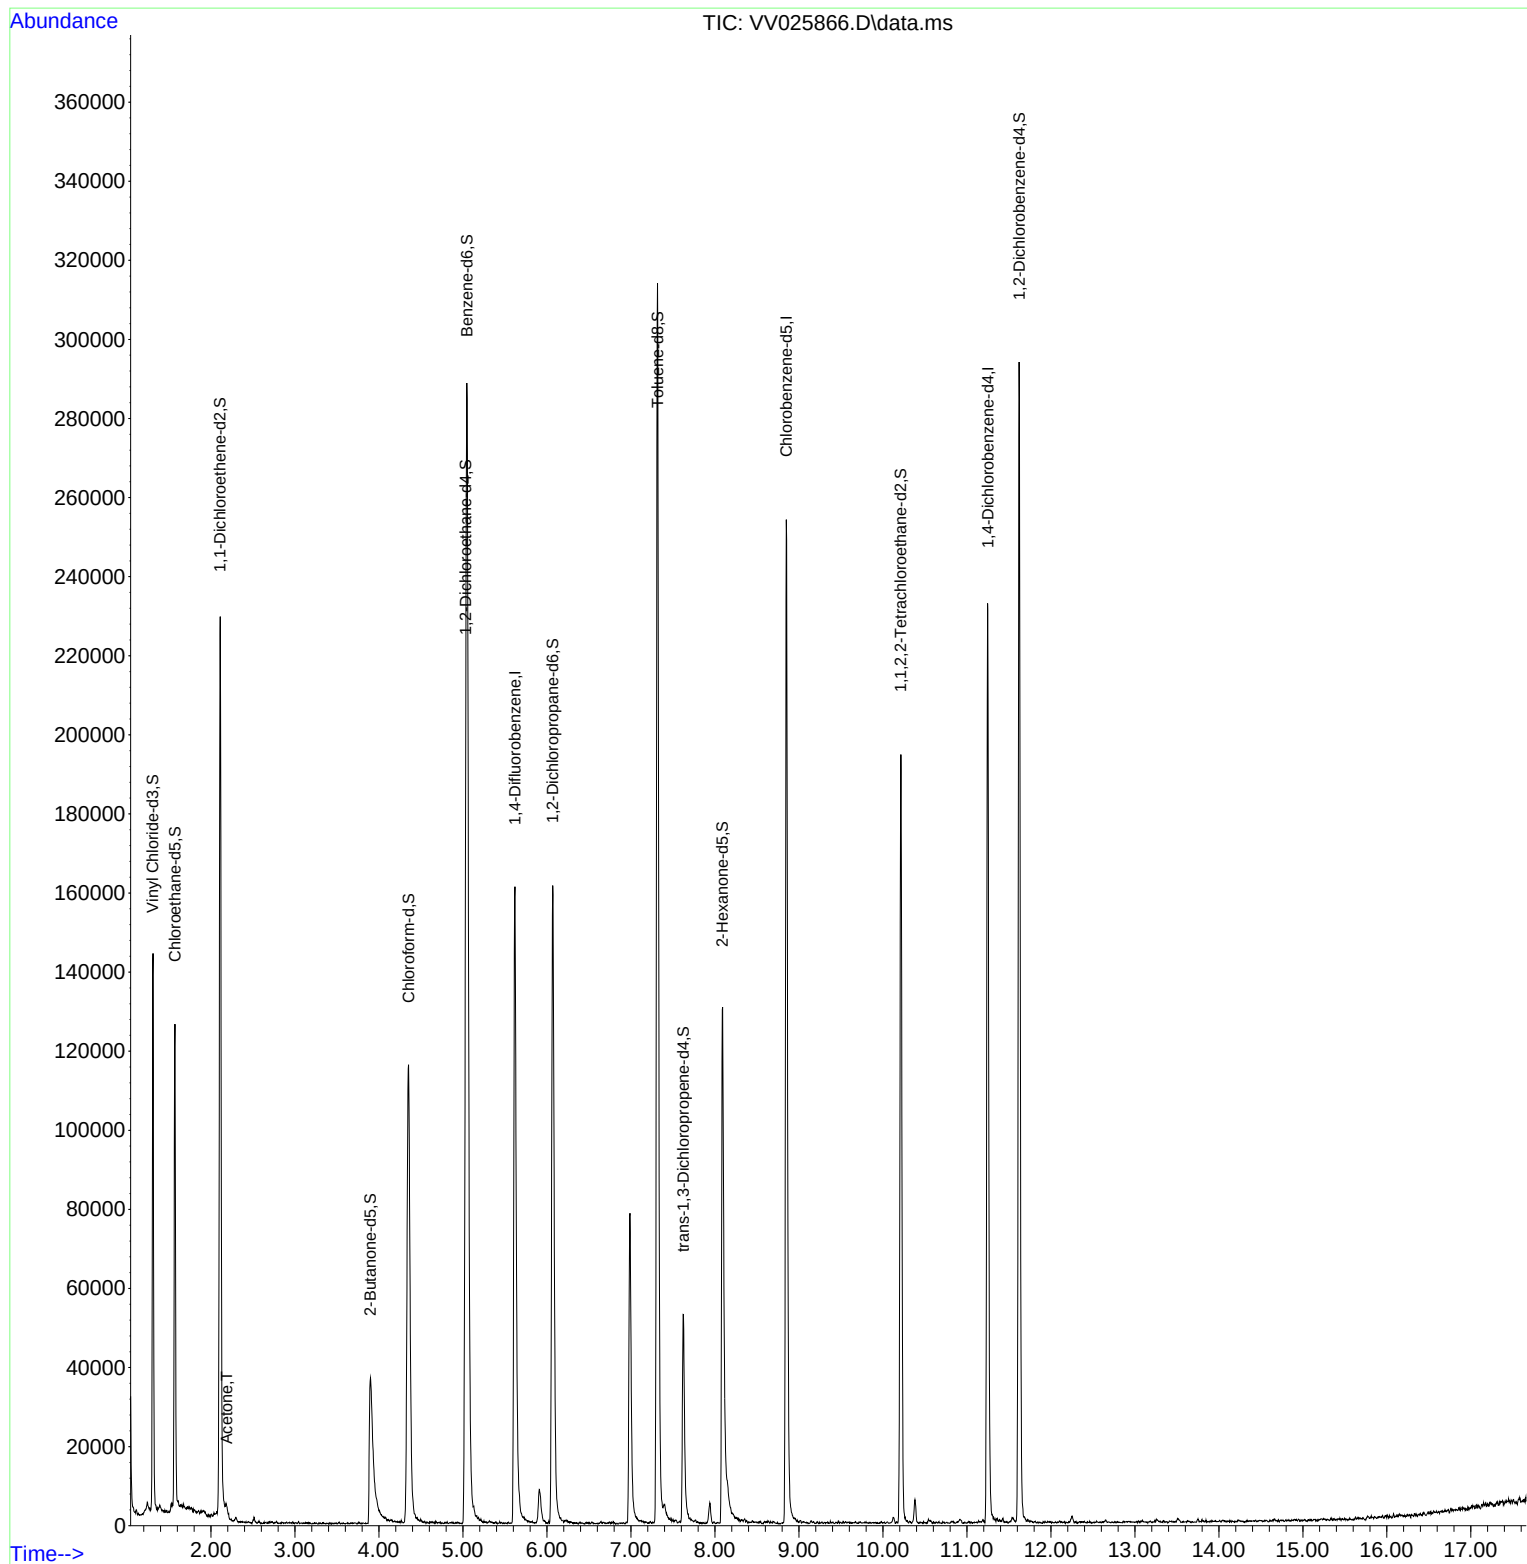

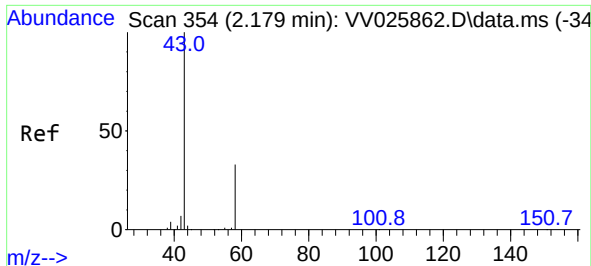

#13
Acetone
Concen: 10.550 ug/L m
RT: 2.188 min Scan# 357
Delta R.T. 0.010 min
Lab File: VV025866.D
Acq: 10 May 2022 17:32

Instrument :
MSVOA_V
ClientSampleId :
DBSK9

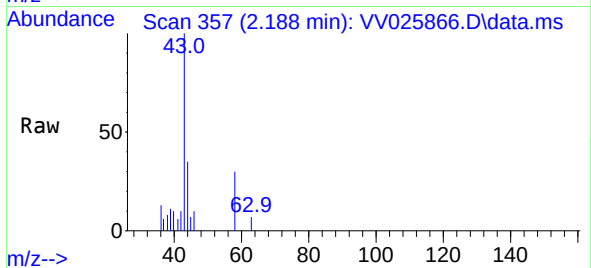

Tgt Ion: 43 Resp: 5570
Ion Ratio Lower Upper
43 100
58 16.6 0.0 65.0

Manual Integrations
APPROVED

Reviewed By :John Carlone 05/18/2022
Supervised By :Mahesh Dadoda 05/18/2022

