

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VW051022\  
 Data File : VW025867.D  
 Acq On : 10 May 2022 17:56  
 Operator : SY/MD  
 Sample : N2713-16  
 Misc : 5mL/MSVOA\_V/WATER  
 ALS Vial : 15 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 DBSL5

Quant Time: May 11 04:25:33 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM051022WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Wed May 11 04:11:56 2022  
 Response via : Initial Calibration


| Compound                      | R.T.    | QIon  | Response | Conc     | Units | Dev(Min)  |
|-------------------------------|---------|-------|----------|----------|-------|-----------|
| -----                         |         |       |          |          |       |           |
| Internal Standards            |         |       |          |          |       |           |
| 1) 1,4-Difluorobenzene        | 5.619   | 114   | 179015   | 50.000   | ug/L  | 0.00      |
| 28) Chlorobenzene-d5          | 8.850   | 117   | 177635   | 50.000   | ug/L  | 0.00      |
| 58) 1,4-Dichlorobenzene-d4    | 11.249  | 152   | 76346    | 50.000   | ug/L  | 0.00      |
| System Monitoring Compounds   |         |       |          |          |       |           |
| 4) Vinyl Chloride-d3          | 1.310   | 65    | 93233    | 40.354   | ug/L  | 0.00      |
| Spiked Amount                 | 50.000  | Range | 60 - 135 | Recovery | =     | 80.700%   |
| 7) Chloroethane-d5            | 1.571   | 69    | 84417    | 41.607   | ug/L  | 0.00      |
| Spiked Amount                 | 50.000  | Range | 70 - 130 | Recovery | =     | 83.220%   |
| 11) 1,1-Dichloroethene-d2     | 2.111   | 63    | 127019   | 31.435   | ug/L  | 0.00      |
| Spiked Amount                 | 50.000  | Range | 60 - 125 | Recovery | =     | 62.860%   |
| 21) 2-Butanone-d5             | 3.896   | 46    | 75354    | 76.096   | ug/L  | 0.01      |
| Spiked Amount                 | 100.000 | Range | 40 - 130 | Recovery | =     | 76.100%   |
| 24) Chloroform-d              | 4.349   | 84    | 127691   | 39.570   | ug/L  | 0.00      |
| Spiked Amount                 | 50.000  | Range | 70 - 125 | Recovery | =     | 79.140%   |
| 26) 1,2-Dichloroethane-d4     | 5.034   | 65    | 84008    | 43.075   | ug/L  | 0.00      |
| Spiked Amount                 | 50.000  | Range | 70 - 125 | Recovery | =     | 86.160%   |
| 32) Benzene-d6                | 5.050   | 84    | 262630   | 42.410   | ug/L  | 0.00      |
| Spiked Amount                 | 50.000  | Range | 70 - 125 | Recovery | =     | 84.820%   |
| 36) 1,2-Dichloropropane-d6    | 6.069   | 67    | 80813    | 42.489   | ug/L  | 0.00      |
| Spiked Amount                 | 50.000  | Range | 70 - 120 | Recovery | =     | 84.980%   |
| 41) Toluene-d8                | 7.317   | 98    | 220388   | 38.626   | ug/L  | 0.00      |
| Spiked Amount                 | 50.000  | Range | 80 - 120 | Recovery | =     | 77.260%#  |
| 43) trans-1,3-Dichloroprop... | 7.625   | 79    | 33572    | 39.541   | ug/L  | 0.00      |
| Spiked Amount                 | 50.000  | Range | 60 - 125 | Recovery | =     | 79.080%   |
| 47) 2-Hexanone-d5             | 8.091   | 63    | 46145    | 66.175   | ug/L  | 0.00      |
| Spiked Amount                 | 100.000 | Range | 45 - 130 | Recovery | =     | 66.170%   |
| 56) 1,1,2,2-Tetrachloroeth... | 10.214  | 84    | 97306    | 38.363   | ug/L  | 0.00      |
| Spiked Amount                 | 50.000  | Range | 65 - 120 | Recovery | =     | 76.720%   |
| 66) 1,2-Dichlorobenzene-d4    | 11.622  | 152   | 77010    | 45.984   | ug/L  | 0.00      |
| Spiked Amount                 | 50.000  | Range | 80 - 120 | Recovery | =     | 91.960%   |
| Target Compounds              |         |       |          |          |       |           |
| 13) Acetone                   | 2.182   | 43    | 5435     | 8.043    | ug/L  | Qvalue 89 |
| -----                         |         |       |          |          |       |           |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV051022\  
Data File : VV025867.D  
Acq On : 10 May 2022 17:56  
Operator : SY/MD  
Sample : N2713-16  
Misc : 5mL/MSVOA\_V/WATER  
ALS Vial : 15 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
DBSL5


Quant Time: May 11 04:25:33 2022  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM051022WMA.M  
Quant Title : VOC Analysis  
QLast Update : Wed May 11 04:11:56 2022  
Response via : Initial Calibration

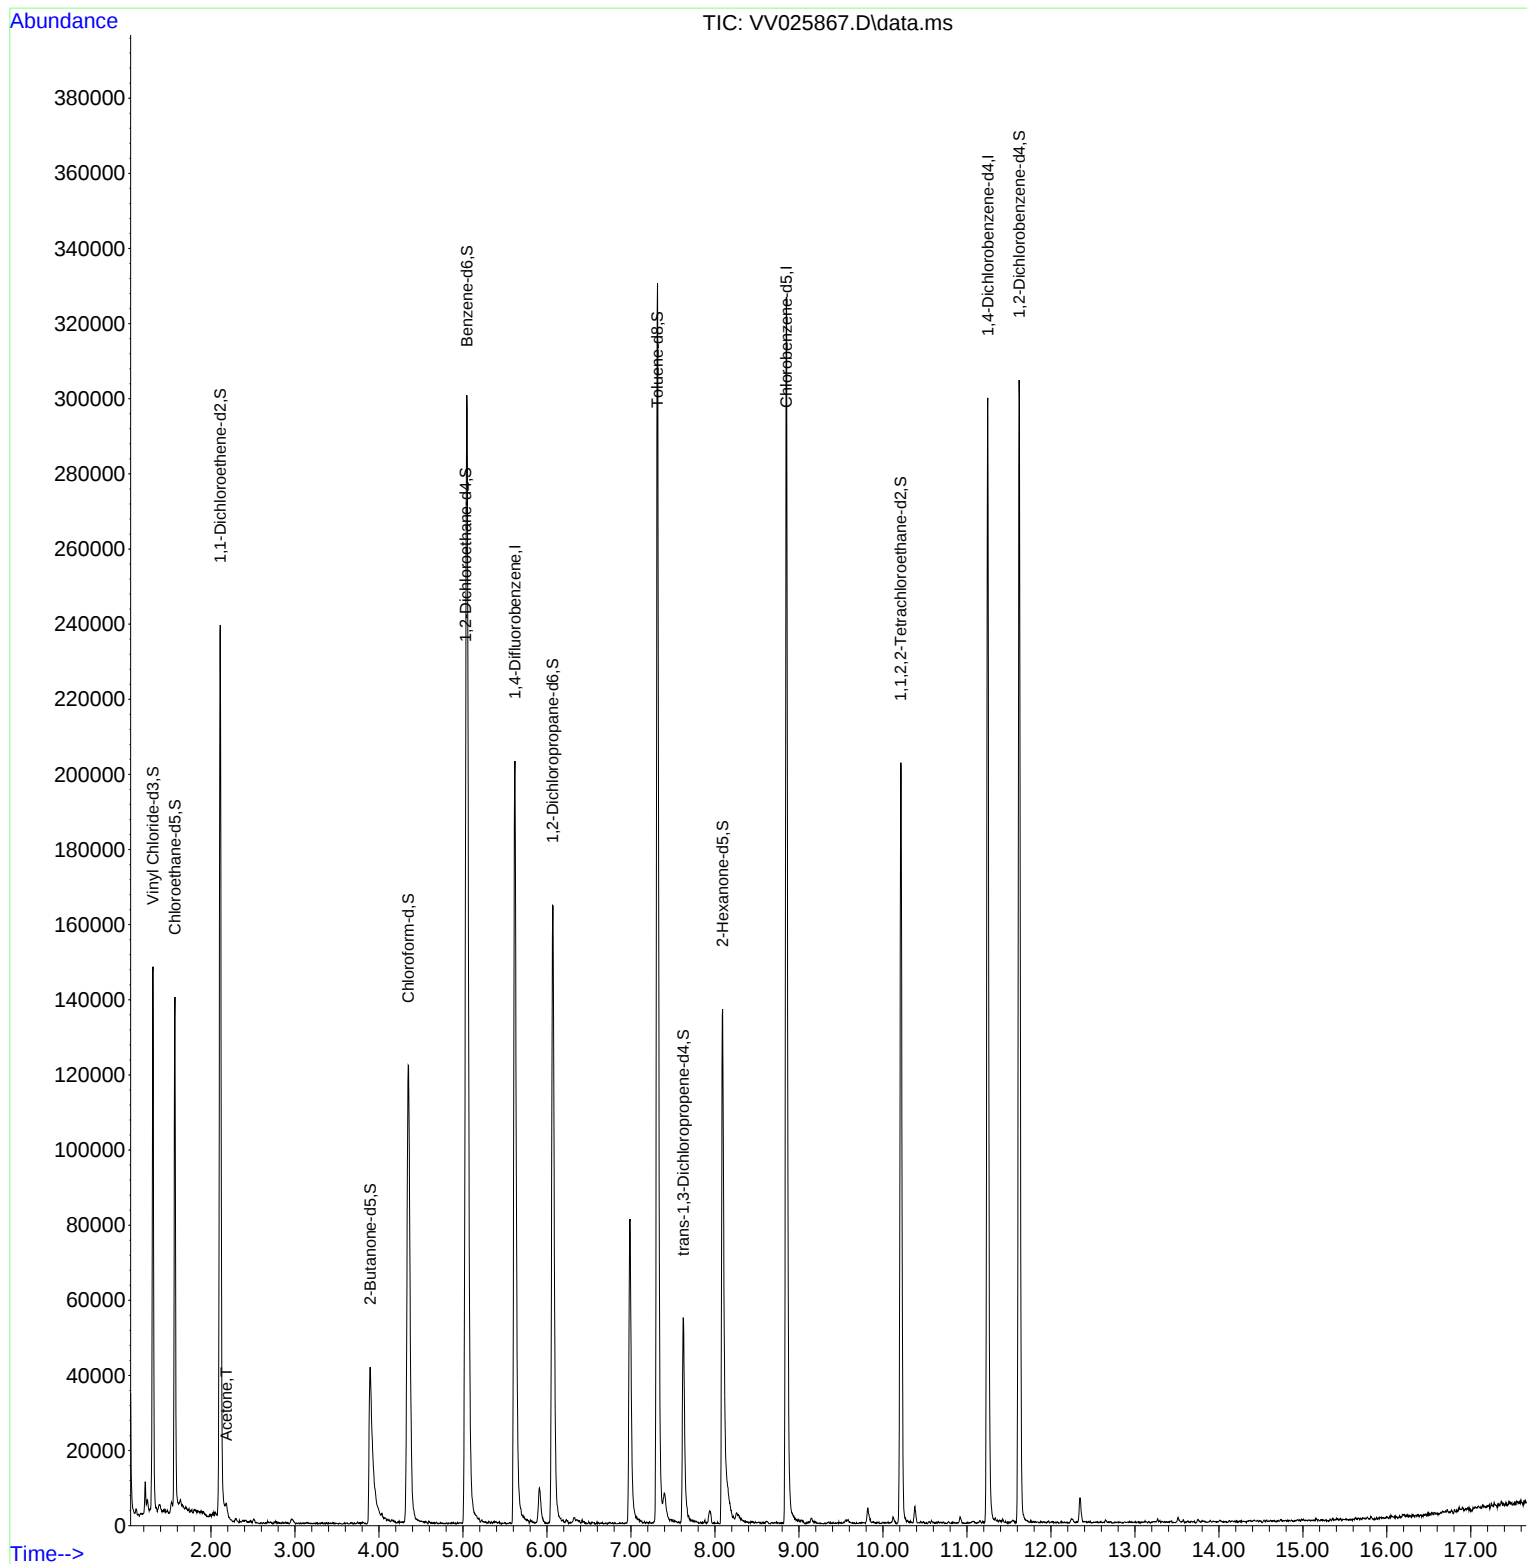

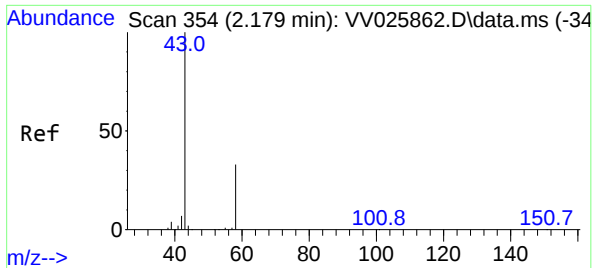

#13  
 Acetone  
 Concen: 8.043 ug/L  
 RT: 2.182 min Scan# 31  
 Delta R.T. 0.003 min  
 Lab File: VV025867.D  
 Acq: 10 May 2022 17:56

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 DBSL5

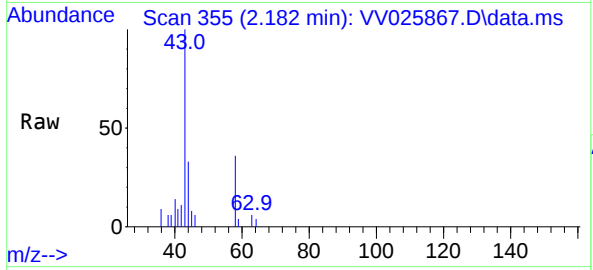

Tgt Ion: 43 Resp: 5435  
 Ion Ratio Lower Upper  
 43 100  
 58 38.6 0.0 65.0

