

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051022\
 Data File : VV025864.D
 Acq On : 10 May 2022 16:45
 Operator : SY/MD
 Sample : VV0510MBL01
 Misc : 5.00g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK212

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

Signal : TIC: VV025864.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	99	rVB	268631	281456	18.51%	2.497%
2	1.571	157	165	177	rBV	218639	250352	16.47%	2.221%
3	2.108	322	332	355	rVB	479100	687543	45.22%	6.100%
4	2.658	501	503	506	rVB	271	145	0.01%	0.001%
5	2.674	506	508	510	rBV2	468	318	0.02%	0.003%
6	2.719	520	522	524	rBV2	302	150	0.01%	0.001%
7	2.761	531	535	537	rBV2	645	578	0.04%	0.005%
8	2.844	553	561	564	rBV4	427	476	0.03%	0.004%
9	2.867	565	568	570	rVV4	483	255	0.02%	0.002%
10	2.886	570	574	579	rVV3	491	359	0.02%	0.003%
11	2.915	579	583	587	rVB3	416	327	0.02%	0.003%
12	2.938	587	590	592	rBV	346	230	0.02%	0.002%
13	2.992	602	607	609	rBV2	627	433	0.03%	0.004%
14	3.066	628	630	635	rVV2	346	274	0.02%	0.002%
15	3.098	635	640	643	rVV3	477	410	0.03%	0.004%
16	3.150	652	656	660	rBV3	459	532	0.03%	0.005%
17	3.188	665	668	671	rBV3	229	162	0.01%	0.001%
18	3.304	702	704	707	rBV	267	203	0.01%	0.002%
19	3.346	714	717	718	rBV2	372	217	0.01%	0.002%
20	3.455	748	751	754	rVV2	254	165	0.01%	0.001%
21	3.507	763	767	768	rBV2	396	307	0.02%	0.003%
22	3.542	775	778	780	rBV2	317	161	0.01%	0.001%
23	3.593	786	794	796	rBV4	465	539	0.04%	0.005%
24	3.648	809	811	814	rVB	319	159	0.01%	0.001%
25	3.777	848	851	854	rVB2	367	182	0.01%	0.002%
26	3.905	877	891	931	rBV2	73845	321961	21.18%	2.856%
27	4.349	1012	1029	1059	rBV	239506	597094	39.27%	5.297%
28	4.584	1100	1102	1107	rVB4	498	435	0.03%	0.004%
29	4.609	1107	1110	1112	rBV2	329	157	0.01%	0.001%
30	4.674	1128	1130	1131	rBV2	343	182	0.01%	0.002%
31	4.757	1153	1156	1157	rBV2	424	202	0.01%	0.002%
32	4.860	1186	1188	1191	rVB2	405	182	0.01%	0.002%
33	4.892	1195	1198	1202	rVB2	247	138	0.01%	0.001%
34	4.944	1211	1214	1216	rBV2	387	254	0.02%	0.002%
35	4.982	1220	1226	1228	rBV4	528	468	0.03%	0.004%
36	5.047	1228	1246	1283	rBV2	596700	1520472	100.00%	13.489%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051022\
 Data File : VV025864.D
 Acq On : 10 May 2022 16:45
 Operator : SY/MD
 Sample : VV0510MBL01
 Misc : 5.00g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK212

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

37	5.616	1411	1423	1450	rBV	388173	787935	51.82%	6.990%
38	5.822	1485	1487	1488	rVB2	506	138	0.01%	0.001%
39	5.908	1503	1514	1525	rBV3	14541	30923	2.03%	0.274%
40	6.069	1547	1564	1598	rBV	330275	683541	44.96%	6.064%
41	6.326	1641	1644	1647	rBV2	462	352	0.02%	0.003%
42	6.484	1691	1693	1696	rVB2	289	135	0.01%	0.001%
43	6.529	1703	1707	1710	rVB2	593	369	0.02%	0.003%
44	6.609	1729	1732	1734	rBV	342	185	0.01%	0.002%
45	6.638	1738	1741	1747	rVB4	382	323	0.02%	0.003%
46	6.696	1756	1759	1761	rBV3	354	254	0.02%	0.002%
47	6.715	1763	1765	1768	rVV2	512	281	0.02%	0.002%
48	6.812	1793	1795	1799	rVB	534	348	0.02%	0.003%
49	6.841	1799	1804	1811	rVB2	512	574	0.04%	0.005%
50	6.870	1811	1813	1816	rBV2	457	302	0.02%	0.003%
51	6.937	1831	1834	1837	rVB3	497	360	0.02%	0.003%
52	6.986	1837	1849	1874	rBV	174348	322677	21.22%	2.863%
53	7.240	1925	1928	1929	rBV2	1021	629	0.04%	0.006%
54	7.314	1940	1951	1972	rBV	695919	1198146	78.80%	10.630%
55	7.622	2037	2047	2070	rBV	118234	214734	14.12%	1.905%
56	7.828	2109	2111	2113	rBV2	517	284	0.02%	0.003%
57	7.908	2134	2136	2139	rBV	495	220	0.01%	0.002%
58	7.976	2154	2157	2158	rBV2	1074	631	0.04%	0.006%
59	8.018	2166	2170	2174	rBV4	618	680	0.04%	0.006%
60	8.088	2181	2192	2234	rBV	326837	659583	43.38%	5.852%
61	8.420	2285	2295	2305	rBV	12660	21972	1.45%	0.195%
62	8.561	2336	2339	2341	rBV2	592	321	0.02%	0.003%
63	8.603	2347	2352	2353	rBV4	535	468	0.03%	0.004%
64	8.686	2375	2378	2381	rBV2	457	286	0.02%	0.003%
65	8.712	2384	2386	2389	rBV3	312	145	0.01%	0.001%
66	8.789	2407	2410	2416	rVB3	356	428	0.03%	0.004%
67	8.850	2416	2429	2452	rBV	623868	1003483	66.00%	8.903%
68	9.371	2583	2591	2592	rBV	530	488	0.03%	0.004%
69	9.622	2667	2669	2671	rBV2	448	218	0.01%	0.002%
70	9.638	2671	2674	2675	rBV	372	166	0.01%	0.001%
71	9.670	2680	2684	2687	rVV3	445	336	0.02%	0.003%
72	9.748	2703	2708	2712	rBV2	405	524	0.03%	0.005%
73	9.805	2724	2726	2729	rVB2	388	146	0.01%	0.001%
74	9.821	2729	2731	2738	rBV3	312	289	0.02%	0.003%
75	9.892	2749	2753	2755	rBV3	398	283	0.02%	0.003%
76	9.931	2761	2765	2767	rBV2	714	563	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051022\
 Data File : VV025864.D
 Acq On : 10 May 2022 16:45
 Operator : SY/MD
 Sample : VV0510MBL01
 Misc : 5.00g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK212

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

77	9.976	2777	2779	2782	rBV	441	266	0.02%	0.002%
78	10.120	2816	2824	2836	rBV7	3055	4807	0.32%	0.043%
79	10.214	2839	2853	2871	rBV	434967	678775	44.64%	6.022%
80	10.490	2936	2939	2944	rBV2	347	262	0.02%	0.002%
81	10.661	2988	2992	2995	rBV2	374	436	0.03%	0.004%
82	10.696	3001	3003	3006	rVB2	635	283	0.02%	0.003%
83	10.728	3009	3013	3014	rBV	385	266	0.02%	0.002%
84	10.770	3024	3026	3029	rBV3	482	211	0.01%	0.002%
85	10.805	3033	3037	3043	rVB6	1872	2116	0.14%	0.019%
86	11.030	3103	3107	3112	rVB5	664	779	0.05%	0.007%
87	11.075	3119	3121	3125	rBV2	378	250	0.02%	0.002%
88	11.133	3137	3139	3140	rBV	561	201	0.01%	0.002%
89	11.185	3150	3155	3158	rBV4	1526	1627	0.11%	0.014%
90	11.246	3163	3174	3202	rVV	609075	938763	61.74%	8.329%
91	11.622	3279	3291	3310	rBV	661915	1021397	67.18%	9.062%
92	11.866	3365	3367	3369	rBV	497	214	0.01%	0.002%
93	11.882	3369	3372	3378	rVB3	700	513	0.03%	0.005%
94	11.992	3403	3406	3408	rBV2	658	449	0.03%	0.004%
95	12.336	3510	3513	3514	rBV3	418	183	0.01%	0.002%
96	12.654	3604	3612	3620	rVB5	2384	3281	0.22%	0.029%
97	12.783	3649	3652	3657	rBV2	400	364	0.02%	0.003%
98	13.178	3772	3775	3778	rBV2	406	308	0.02%	0.003%
99	13.506	3871	3877	3888	rBV3	6517	9697	0.64%	0.086%
100	13.747	3946	3952	3960	rVB5	3590	4915	0.32%	0.044%




Sum of corrected areas: 11271561

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051022\
Data File : VV025864.D
Acq On : 10 May 2022 16:45
Operator : SY/MD
Sample : VV0510MBL01
Misc : 5.00g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK212

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

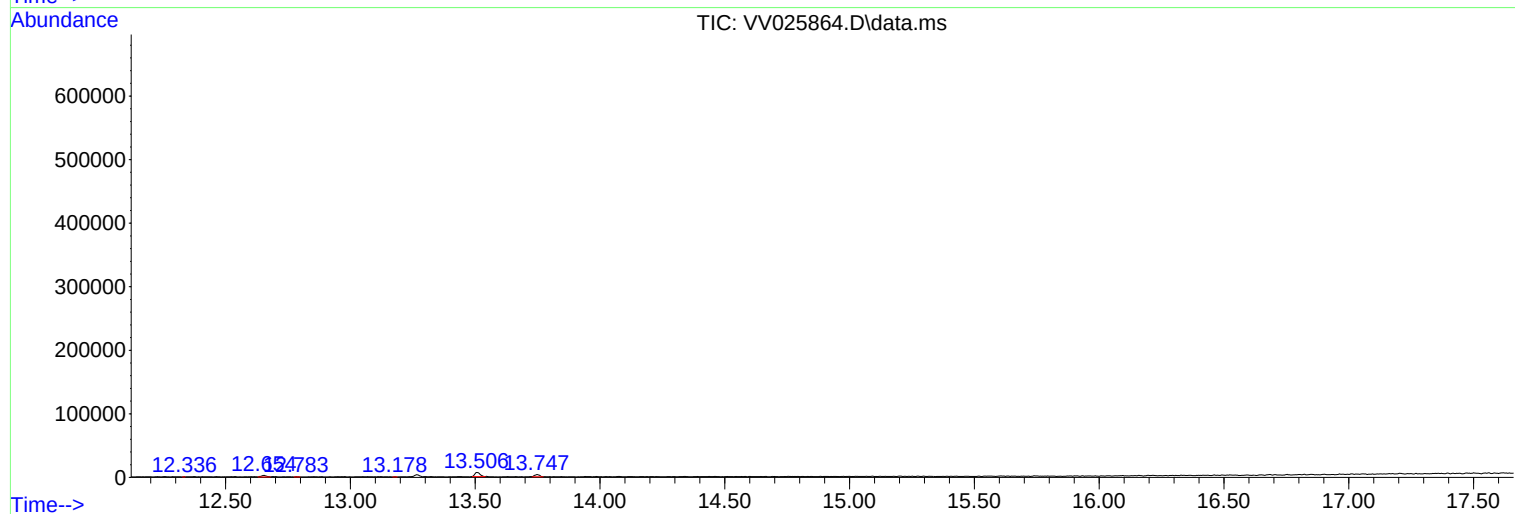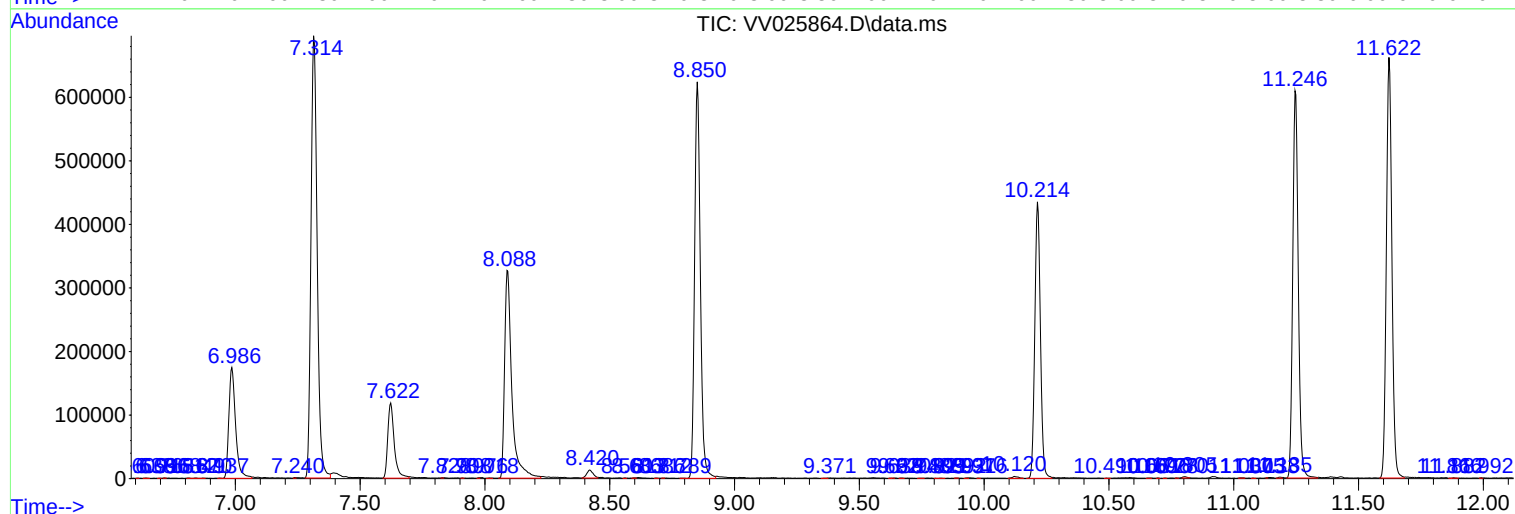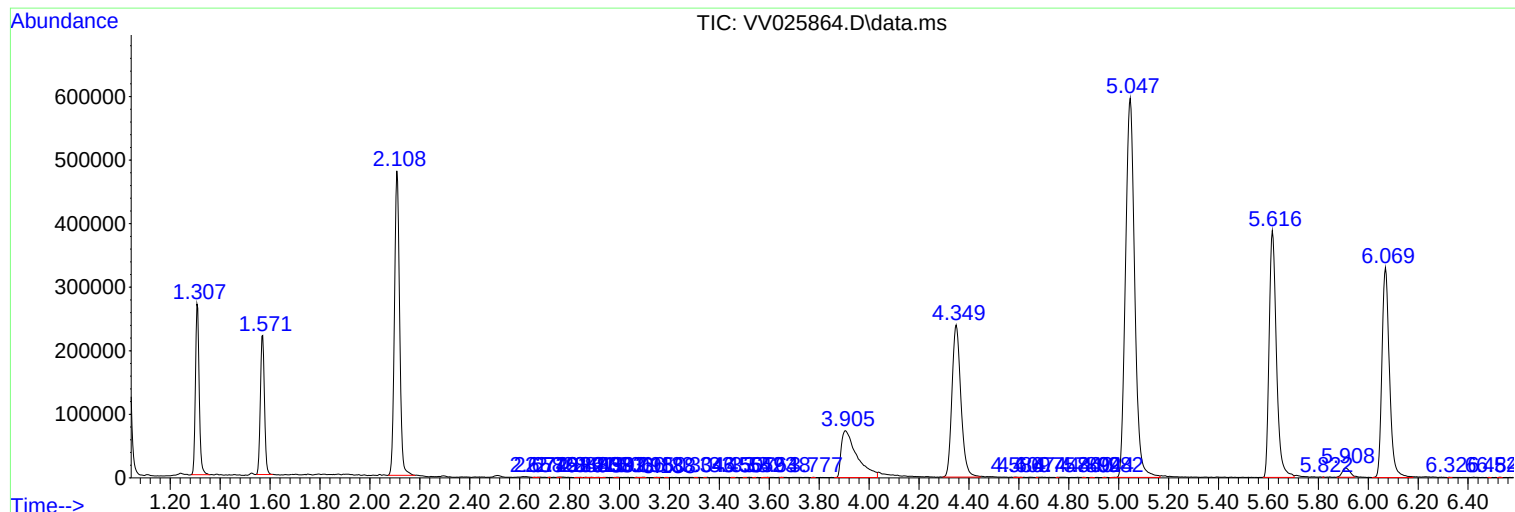

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051022\
Data File : VV025864.D
Acq On : 10 May 2022 16:45
Operator : SY/MD
Sample : VV0510MBL01
Misc : 5.00g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK212

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051022\
Data File : VV025864.D
Acq On : 10 May 2022 16:45
Operator : SY/MD
Sample : VV0510MBL01
Misc : 5.00g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK212

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc