

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051022\
 Data File : VV025867.D
 Acq On : 10 May 2022 17:56
 Operator : SY/MD
 Sample : N2713-16
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBSL5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

Signal : TIC: VV025867.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	75	84	95	rBV	144411	158406	20.65%	2.813%
2	1.571	158	165	178	rVB	134918	148294	19.34%	2.633%
3	2.111	323	333	350	rBV	236061	344340	44.90%	6.114%
4	2.339	402	404	406	rBV2	769	327	0.04%	0.006%
5	2.507	451	456	465	rVB6	1087	1594	0.21%	0.028%
6	2.625	490	493	496	rVB3	337	210	0.03%	0.004%
7	2.674	506	508	510	rBV	531	211	0.03%	0.004%
8	2.761	530	535	536	rBV3	536	399	0.05%	0.007%
9	2.847	559	562	565	rBV2	461	284	0.04%	0.005%
10	2.918	580	584	588	rVB2	324	263	0.03%	0.005%
11	2.957	588	596	612	rVB7	1328	3279	0.43%	0.058%
12	3.018	612	615	618	rBV2	294	241	0.03%	0.004%
13	3.069	627	631	633	rBV2	299	160	0.02%	0.003%
14	3.105	639	642	645	rVB2	318	210	0.03%	0.004%
15	3.121	645	647	650	rBV2	287	171	0.02%	0.003%
16	3.137	650	652	655	rVV3	302	205	0.03%	0.004%
17	3.262	688	691	695	rVB2	354	243	0.03%	0.004%
18	3.371	723	725	728	rBV2	430	240	0.03%	0.004%
19	3.394	731	732	735	rBV	395	206	0.03%	0.004%
20	3.426	740	742	746	rVB	267	164	0.02%	0.003%
21	3.465	751	754	757	rVB2	355	200	0.03%	0.004%
22	3.529	771	774	780	rBV2	281	272	0.04%	0.005%
23	3.744	838	841	844	rVV3	422	249	0.03%	0.004%
24	3.789	852	855	857	rBV4	357	245	0.03%	0.004%
25	3.896	876	888	928	rBV	41745	133345	17.39%	2.368%
26	4.349	1015	1029	1057	rBV	121271	307934	40.15%	5.468%
27	4.545	1088	1090	1092	rBV	397	200	0.03%	0.004%
28	4.593	1102	1105	1112	rBV7	798	880	0.11%	0.016%
29	4.809	1167	1172	1174	rVB2	347	281	0.04%	0.005%
30	4.860	1185	1188	1190	rVB	337	160	0.02%	0.003%
31	4.934	1208	1211	1214	rBV2	408	260	0.03%	0.005%
32	5.047	1229	1246	1274	rBV2	300356	766961	100.00%	13.618%
33	5.307	1324	1327	1333	rVB2	648	543	0.07%	0.010%
34	5.619	1413	1424	1450	rBV	202920	421847	55.00%	7.490%
35	5.802	1477	1481	1484	rBV4	907	687	0.09%	0.012%
36	5.870	1498	1502	1503	rBV2	337	236	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051022\
 Data File : VV025867.D
 Acq On : 10 May 2022 17:56
 Operator : SY/MD
 Sample : N2713-16
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBSL5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

37	5.912	1505	1515	1532	rVV3	9244	19776	2.58%	0.351%
38	6.024	1546	1550	1551	rBV2	395	247	0.03%	0.004%
39	6.069	1551	1564	1586	rBV	164383	344934	44.97%	6.125%
40	6.420	1670	1673	1675	rBV2	790	378	0.05%	0.007%
41	6.497	1694	1697	1699	rBV2	529	284	0.04%	0.005%
42	6.535	1706	1709	1713	rBV3	548	423	0.06%	0.008%
43	6.596	1725	1728	1730	rVB2	521	203	0.03%	0.004%
44	6.612	1730	1733	1734	rBV2	333	165	0.02%	0.003%
45	6.645	1737	1743	1748	rBV2	315	381	0.05%	0.007%
46	6.699	1754	1760	1762	rBV	249	177	0.02%	0.003%
47	6.728	1766	1769	1770	rBV	300	160	0.02%	0.003%
48	6.747	1774	1775	1783	rVB3	341	251	0.03%	0.004%
49	6.780	1783	1785	1789	rVB2	401	295	0.04%	0.005%
50	6.805	1789	1793	1795	rBV2	360	248	0.03%	0.004%
51	6.931	1828	1832	1835	rBV2	296	301	0.04%	0.005%
52	6.989	1838	1850	1873	rBV	80969	155645	20.29%	2.764%
53	7.188	1908	1912	1914	rBV3	350	284	0.04%	0.005%
54	7.223	1919	1923	1925	rBV3	530	377	0.05%	0.007%
55	7.317	1941	1952	1970	rBV	329358	574798	74.94%	10.206%
56	7.564	2026	2029	2033	rBV3	369	214	0.03%	0.004%
57	7.622	2038	2047	2065	rBV	54507	100932	13.16%	1.792%
58	7.850	2113	2118	2120	rBV3	503	304	0.04%	0.005%
59	7.937	2138	2145	2157	rVB4	3389	6409	0.84%	0.114%
60	7.992	2160	2162	2164	rVB2	418	167	0.02%	0.003%
61	8.091	2183	2193	2230	rBV	136995	286862	37.40%	5.094%
62	8.429	2296	2298	2299	rBV	457	176	0.02%	0.003%
63	8.548	2332	2335	2337	rVB2	418	163	0.02%	0.003%
64	8.612	2350	2355	2358	rBV4	583	653	0.09%	0.012%
65	8.673	2370	2374	2377	rBV2	425	393	0.05%	0.007%
66	8.735	2391	2393	2396	rVB2	460	212	0.03%	0.004%
67	8.850	2419	2429	2450	rBV	326463	534555	69.70%	9.492%
68	9.088	2500	2503	2505	rBV3	430	229	0.03%	0.004%
69	9.104	2505	2508	2510	rBV2	435	270	0.04%	0.005%
70	9.146	2516	2521	2522	rBV2	1093	927	0.12%	0.016%
71	9.201	2535	2538	2542	rVB3	473	327	0.04%	0.006%
72	9.342	2577	2582	2583	rBV2	333	278	0.04%	0.005%
73	9.407	2599	2602	2604	rBV2	414	252	0.03%	0.004%
74	9.532	2636	2641	2642	rBV	397	258	0.03%	0.005%
75	9.661	2678	2681	2685	rVB2	341	233	0.03%	0.004%
76	9.686	2685	2689	2691	rBV2	392	213	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051022\
 Data File : VV025867.D
 Acq On : 10 May 2022 17:56
 Operator : SY/MD
 Sample : N2713-16
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBSL5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

77	9.821	2722	2731	2745	rBV6	4117	7499	0.98%	0.133%
78	10.214	2838	2853	2869	rBV	202647	322318	42.03%	5.723%
79	10.381	2898	2905	2915	rVB	4394	6039	0.79%	0.107%
80	10.448	2924	2926	2933	rVV2	457	349	0.05%	0.006%
81	10.487	2933	2938	2940	rVB2	407	319	0.04%	0.006%
82	10.548	2951	2957	2959	rBV3	603	595	0.08%	0.011%
83	10.577	2963	2966	2972	rBV3	699	725	0.09%	0.013%
84	10.625	2980	2981	2984	rBV2	302	168	0.02%	0.003%
85	10.661	2988	2992	2994	rBV	456	265	0.03%	0.005%
86	10.831	3042	3045	3046	rBV	470	190	0.02%	0.003%
87	11.005	3096	3099	3101	rBV	371	160	0.02%	0.003%
88	11.120	3132	3135	3138	rBV2	279	214	0.03%	0.004%
89	11.249	3164	3175	3197	rBV	299340	467078	60.90%	8.293%
90	11.461	3239	3241	3245	rVB4	545	250	0.03%	0.004%
91	11.509	3253	3256	3258	rBV2	364	242	0.03%	0.004%
92	11.622	3280	3291	3315	rBV	304113	486487	63.43%	8.638%
93	11.757	3331	3333	3336	rVB4	575	218	0.03%	0.004%
94	11.773	3336	3338	3341	rVB2	391	168	0.02%	0.003%
95	12.307	3501	3504	3507	rBV	369	241	0.03%	0.004%
96	12.345	3509	3516	3527	rVB7	6511	10318	1.35%	0.183%
97	12.593	3591	3593	3596	rBV	396	192	0.03%	0.003%
98	13.004	3719	3721	3724	rVB	454	225	0.03%	0.004%
99	13.416	3847	3849	3852	rBV	366	280	0.04%	0.005%
100	14.336	4132	4135	4136	rBV2	433	267	0.03%	0.005%




Sum of corrected areas: 5631908

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051022\
Data File : VV025867.D
Acq On : 10 May 2022 17:56
Operator : SY/MD
Sample : N2713-16
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBSL5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

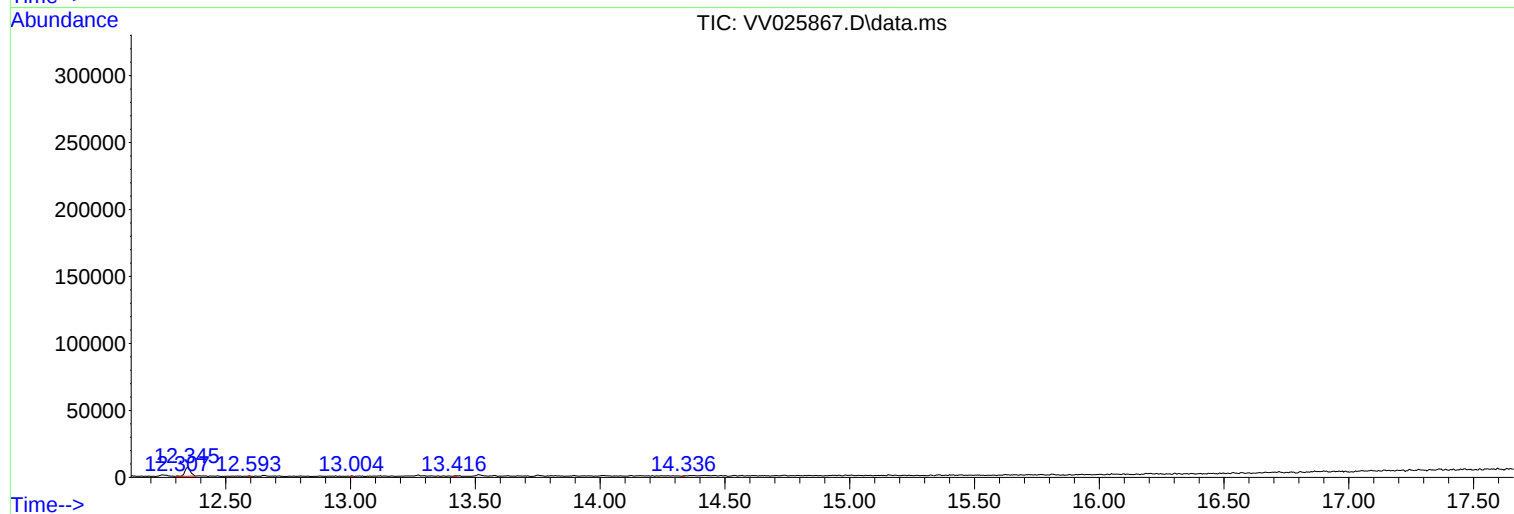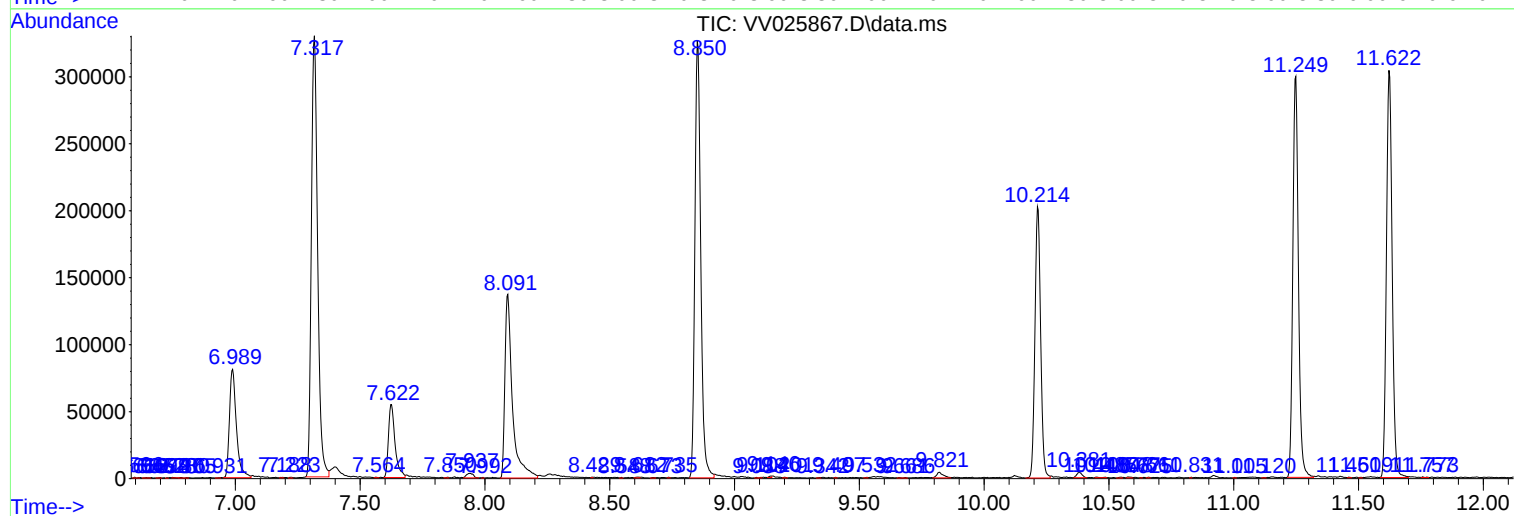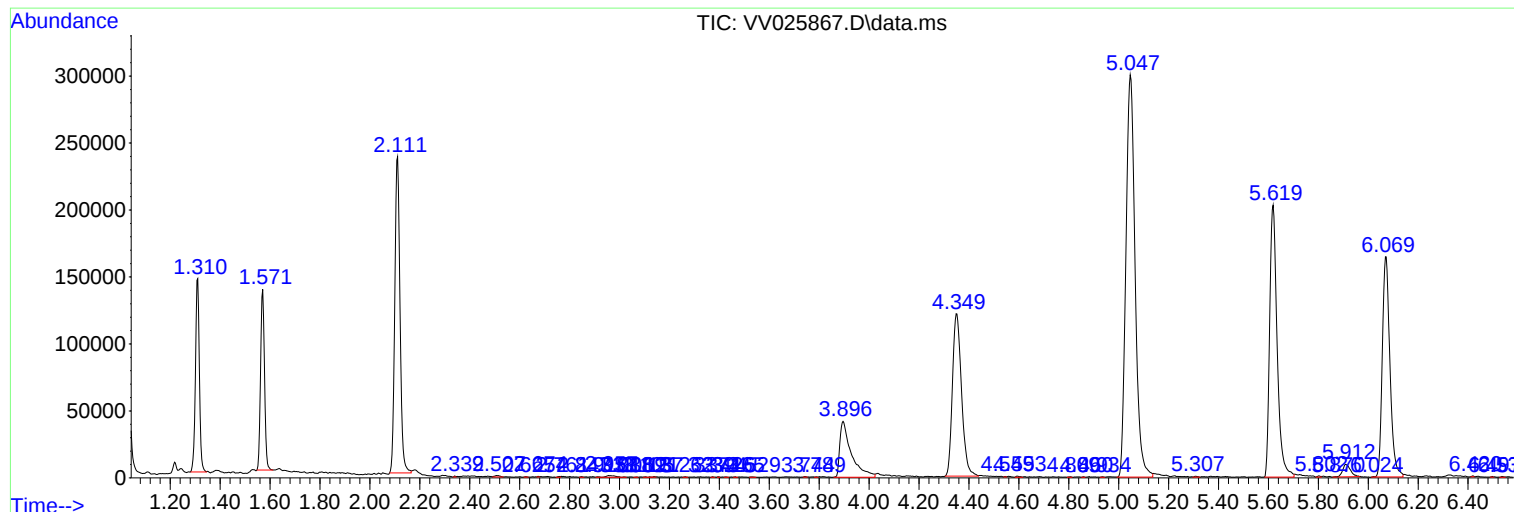

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051022\
Data File : VV025867.D
Acq On : 10 May 2022 17:56
Operator : SY/MD
Sample : N2713-16
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBSL5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051022\
Data File : VV025867.D
Acq On : 10 May 2022 17:56
Operator : SY/MD
Sample : N2713-16
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBSL5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
