

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051022\
 Data File : VV025868.D
 Acq On : 10 May 2022 18:20
 Operator : SY/MD
 Sample : N2713-10
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

Signal : TIC: VV025868.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.311	77	84	100	rVB	95487	99928	20.39%	2.802%
2	1.571	158	165	173	rVB	83372	91311	18.63%	2.561%
3	2.111	323	333	343	rBV	151655	220194	44.93%	6.175%
4	2.433	431	433	434	rBV	645	191	0.04%	0.005%
5	2.446	434	437	441	rVB2	836	564	0.12%	0.016%
6	2.465	441	443	444	rBV	490	202	0.04%	0.006%
7	2.513	449	458	468	rVB6	2609	4196	0.86%	0.118%
8	2.577	475	478	481	rBV3	597	359	0.07%	0.010%
9	2.677	507	509	511	rVB2	512	224	0.05%	0.006%
10	2.757	528	534	536	rBV2	427	425	0.09%	0.012%
11	2.812	549	551	557	rVB2	305	244	0.05%	0.007%
12	2.844	557	561	564	rBV3	334	284	0.06%	0.008%
13	3.111	640	644	648	rBV2	380	314	0.06%	0.009%
14	3.220	673	678	679	rBV	294	203	0.04%	0.006%
15	3.301	700	703	704	rBV	364	204	0.04%	0.006%
16	3.407	732	736	737	rBV2	382	271	0.06%	0.008%
17	3.577	783	789	792	rBV2	399	337	0.07%	0.009%
18	3.738	835	839	841	rBV3	387	271	0.06%	0.008%
19	3.851	872	874	876	rVB	440	170	0.03%	0.005%
20	3.905	879	891	920	rBV2	29157	103873	21.20%	2.913%
21	4.352	1017	1030	1055	rVB	78723	193332	39.45%	5.422%
22	4.613	1106	1111	1113	rBV	248	195	0.04%	0.005%
23	4.629	1113	1116	1118	rBV2	357	183	0.04%	0.005%
24	4.671	1124	1129	1132	rBV2	284	334	0.07%	0.009%
25	4.699	1136	1138	1142	rVB2	473	267	0.05%	0.007%
26	4.748	1149	1153	1156	rBV2	321	240	0.05%	0.007%
27	4.838	1177	1181	1184	rVB3	459	336	0.07%	0.009%
28	4.896	1196	1199	1204	rVB	317	217	0.04%	0.006%
29	4.921	1204	1207	1210	rBV3	364	212	0.04%	0.006%
30	5.047	1231	1246	1274	rBV2	189513	490036	100.00%	13.742%
31	5.233	1302	1304	1307	rVB2	577	376	0.08%	0.011%
32	5.304	1323	1326	1328	rBV	392	244	0.05%	0.007%
33	5.468	1376	1377	1381	rVV2	357	231	0.05%	0.006%
34	5.542	1398	1400	1402	rBV	466	192	0.04%	0.005%
35	5.564	1405	1407	1411	rVB2	309	236	0.05%	0.007%
36	5.619	1411	1424	1449	rBV	129398	266603	54.40%	7.476%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051022\
 Data File : VV025868.D
 Acq On : 10 May 2022 18:20
 Operator : SY/MD
 Sample : N2713-10
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

37	5.834	1486	1491	1493	rBV2	323	276	0.06%	0.008%
38	5.870	1500	1502	1503	rBV2	418	176	0.04%	0.005%
39	5.912	1508	1515	1526	rVV6	4176	7437	1.52%	0.209%
40	6.069	1551	1564	1592	rBV	106559	225202	45.96%	6.315%
41	6.201	1604	1605	1607	rBV	549	187	0.04%	0.005%
42	6.240	1614	1617	1619	rBV2	659	417	0.09%	0.012%
43	6.474	1685	1690	1692	rVV2	531	474	0.10%	0.013%
44	6.571	1715	1720	1725	rBV2	419	376	0.08%	0.011%
45	6.603	1725	1730	1734	rVV3	485	332	0.07%	0.009%
46	6.687	1753	1756	1758	rVB2	341	191	0.04%	0.005%
47	6.709	1758	1763	1767	rBV2	300	275	0.06%	0.008%
48	6.831	1798	1801	1805	rVV2	395	264	0.05%	0.007%
49	6.989	1840	1850	1874	rBV	48417	94810	19.35%	2.659%
50	7.195	1912	1914	1917	rBV2	309	177	0.04%	0.005%
51	7.240	1927	1928	1930	rVB2	517	174	0.04%	0.005%
52	7.262	1931	1935	1936	rBV	334	214	0.04%	0.006%
53	7.317	1941	1952	1976	rBV	198991	356914	72.83%	10.009%
54	7.513	2009	2013	2014	rBV2	257	198	0.04%	0.006%
55	7.625	2039	2048	2070	rBV2	33424	63528	12.96%	1.782%
56	7.876	2123	2126	2131	rVB3	498	406	0.08%	0.011%
57	7.937	2138	2145	2152	rBV6	1429	1996	0.41%	0.056%
58	8.092	2184	2193	2234	rBV	83711	176682	36.05%	4.955%
59	8.423	2287	2296	2313	rVB3	5596	10294	2.10%	0.289%
60	8.487	2313	2316	2318	rBV	384	170	0.03%	0.005%
61	8.545	2331	2334	2335	rBV	414	274	0.06%	0.008%
62	8.616	2352	2356	2360	rBV	538	498	0.10%	0.014%
63	8.725	2388	2390	2394	rVB	565	291	0.06%	0.008%
64	8.793	2409	2411	2413	rBV2	299	199	0.04%	0.006%
65	8.854	2419	2430	2455	rBV	207113	336399	68.65%	9.434%
66	9.114	2508	2511	2514	rBV2	484	344	0.07%	0.010%
67	9.146	2519	2521	2523	rBV2	309	181	0.04%	0.005%
68	9.288	2560	2565	2567	rBV	469	359	0.07%	0.010%
69	9.384	2591	2595	2597	rBV3	440	286	0.06%	0.008%
70	9.416	2602	2605	2608	rBV	480	391	0.08%	0.011%
71	9.484	2622	2626	2627	rBV3	262	185	0.04%	0.005%
72	9.680	2685	2687	2692	rVB2	387	179	0.04%	0.005%
73	9.764	2709	2713	2716	rBV3	394	301	0.06%	0.008%
74	9.809	2724	2727	2728	rBV	336	183	0.04%	0.005%
75	9.854	2738	2741	2746	rBV	381	297	0.06%	0.008%
76	9.911	2756	2759	2762	rBV	418	341	0.07%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051022\
 Data File : VV025868.D
 Acq On : 10 May 2022 18:20
 Operator : SY/MD
 Sample : N2713-10
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis

77	9.966	2773	2776	2778	rBV	299	179	0.04%	0.005%
78	10.088	2811	2814	2819	rVB2	345	300	0.06%	0.008%
79	10.114	2819	2822	2823	rBV2	692	339	0.07%	0.010%
80	10.175	2837	2841	2842	rBV	376	178	0.04%	0.005%
81	10.214	2842	2853	2873	rVV	134221	212962	43.46%	5.972%
82	10.384	2900	2906	2907	rBV3	913	748	0.15%	0.021%
83	10.477	2932	2935	2937	rBV2	279	181	0.04%	0.005%
84	10.583	2962	2968	2970	rBV4	433	485	0.10%	0.014%
85	10.911	3066	3070	3072	rBV2	494	427	0.09%	0.012%
86	11.040	3108	3110	3112	rBV2	309	194	0.04%	0.005%
87	11.249	3160	3175	3196	rBV	188356	292250	59.64%	8.196%
88	11.497	3249	3252	3255	rBV2	448	299	0.06%	0.008%
89	11.622	3281	3291	3308	rBV	185589	295030	60.21%	8.274%
90	11.802	3341	3347	3350	rBV3	476	444	0.09%	0.012%
91	12.198	3468	3470	3473	rBV2	358	237	0.05%	0.007%
92	12.355	3516	3519	3522	rBV2	375	234	0.05%	0.007%
93	12.381	3525	3527	3531	rVV	465	231	0.05%	0.006%
94	12.622	3597	3602	3603	rBV2	429	349	0.07%	0.010%
95	13.152	3765	3767	3769	rBV	451	267	0.05%	0.007%
96	13.374	3834	3836	3839	rBV2	333	177	0.04%	0.005%
97	13.747	3950	3952	3956	rVB2	778	399	0.08%	0.011%
98	13.847	3980	3983	3986	rBV2	639	484	0.10%	0.014%
99	14.442	4166	4168	4169	rBV	591	281	0.06%	0.008%
100	14.500	4184	4186	4189	rBV3	528	344	0.07%	0.010%




Sum of corrected areas: 3565896

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051022\
Data File : VV025868.D
Acq On : 10 May 2022 18:20
Operator : SY/MD
Sample : N2713-10
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

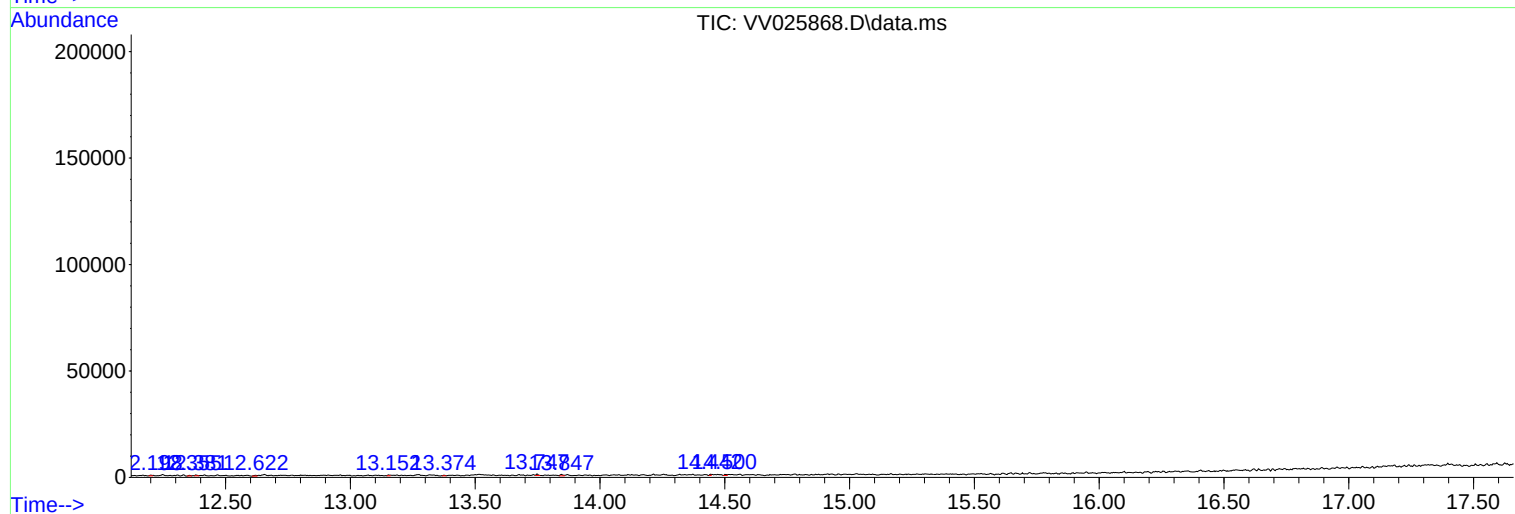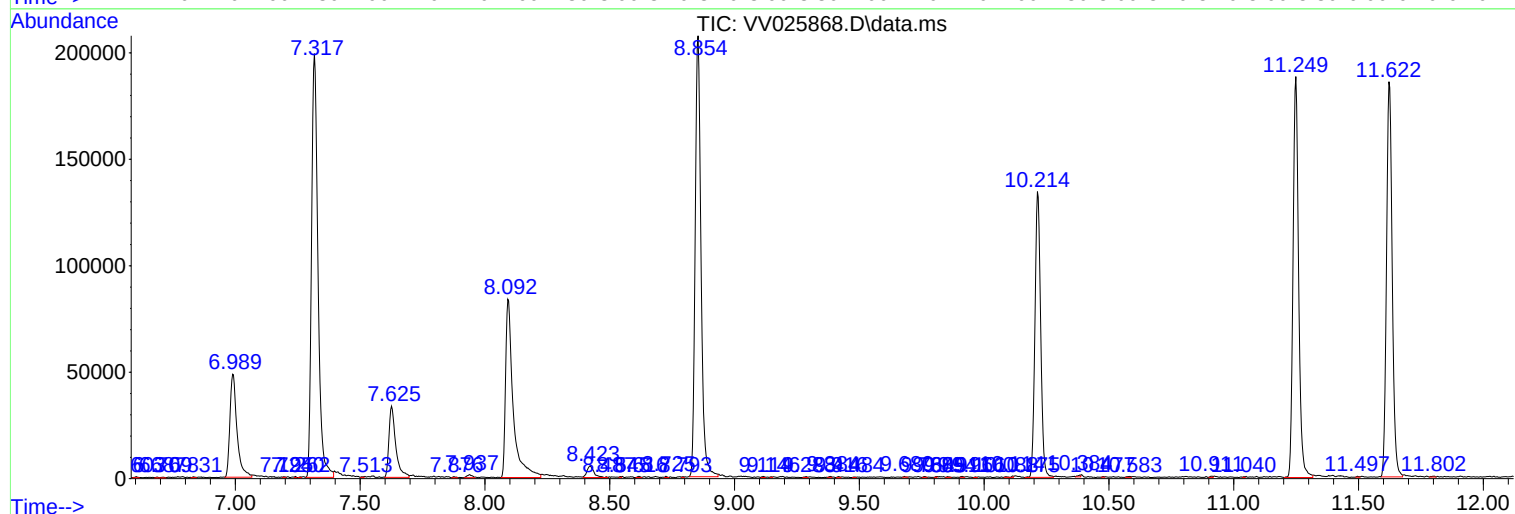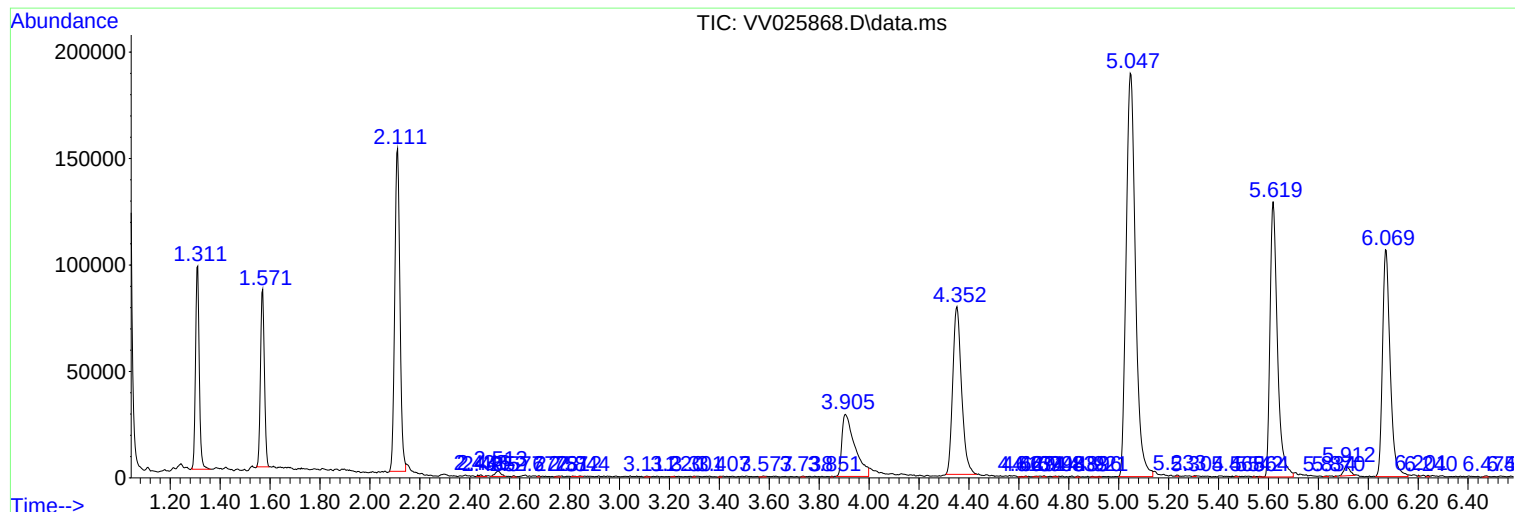

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051022\
Data File : VV025868.D
Acq On : 10 May 2022 18:20
Operator : SY/MD
Sample : N2713-10
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051022\
Data File : VV025868.D
Acq On : 10 May 2022 18:20
Operator : SY/MD
Sample : N2713-10
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------