


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051022\
 Data File : VV025855.D
 Acq On : 10 May 2022 10:06
 Operator : SY/MD
 Sample : BFB281
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB281

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051022WMA.M
 Title : VOC Analysis
 Last Update : Fri May 13 07:07:32 2022

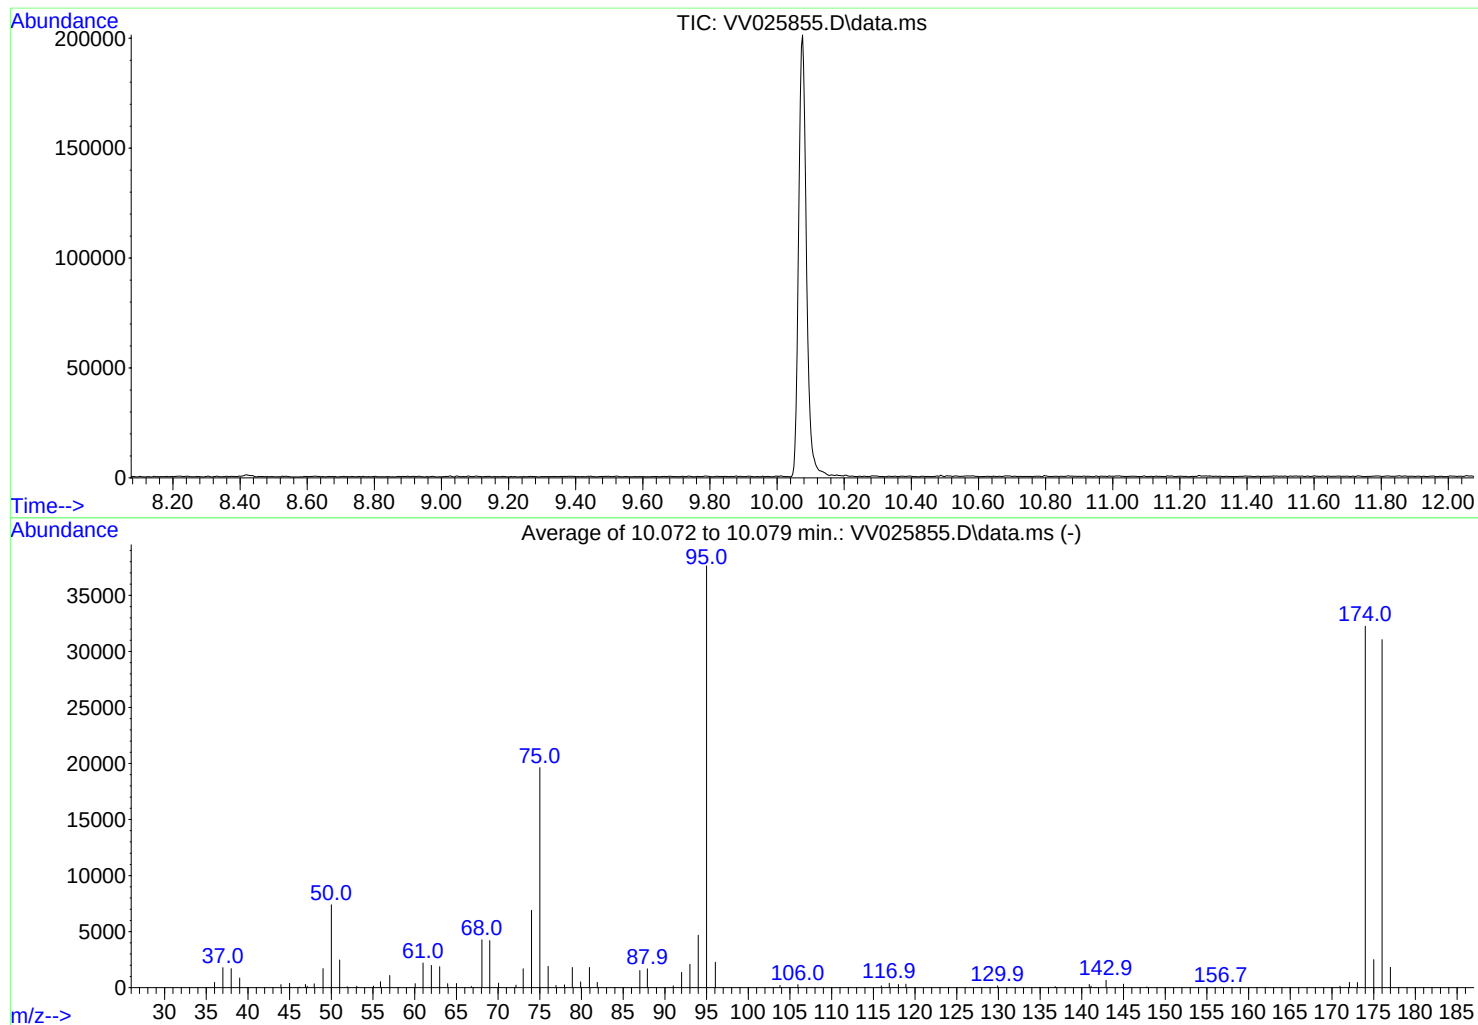

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2798

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	7396	PASS
75	95	30	80	52.2	19635	PASS
95	95	100	100	100.0	37637	PASS
96	95	5	9	6.0	2275	PASS
173	174	0.00	2	1.4	463	PASS
174	95	50	120	85.7	32251	PASS
175	174	5	9	7.8	2500	PASS
176	174	95	105	96.3	31053	PASS
177	176	5	10	5.9	1820	PASS

m/z	Abundance
39.90	263.0
44.00	283.0

Instrument :
MSVOA_V
ClientSampleId :
BFB281

m/z	Abundance
36.00	472.0
37.00	1776.0
38.00	1695.0
39.00	899.0
39.90	288.0
44.00	542.0
45.00	379.0
46.20	124.0
46.90	418.0
48.00	353.0
49.00	1889.0
50.00	7562.0
51.00	2449.0
53.00	148.0
55.00	132.0
55.90	523.0
57.00	1095.0
60.00	409.0
61.00	2181.0
62.00	2069.0
63.00	2008.0
63.90	332.0
65.00	317.0
66.80	167.0
68.00	4315.0
69.00	4216.0
70.00	388.0
72.20	197.0
73.00	1713.0
74.00	6959.0
75.00	19880.0
76.00	1809.0
76.90	211.0
78.00	219.0
78.90	1765.0
79.90	486.0
80.90	1745.0
81.90	491.0
87.00	1549.0
87.90	1639.0
91.00	151.0
92.00	1459.0
93.00	1943.0
94.00	4829.0
95.00	37864.0
96.10	2381.0
103.80	199.0
105.90	209.0
115.90	165.0
116.90	388.0
118.00	307.0
118.90	327.0
129.90	151.0
140.90	443.0
141.70	105.0
142.90	698.0
145.00	318.0
147.80	108.0
170.90	144.0
172.10	467.0
173.00	448.0
174.00	32176.0
175.00	2462.0
176.00	31064.0
177.00	1676.0

Instrument :
MSVOA_V
ClientSampleId :
BFB281

m/z	Abundance
36.00	486.0
37.00	1828.0
38.00	1753.0
39.00	891.0
39.90	301.0
43.90	551.0
45.00	384.0
46.90	436.0
47.90	365.0
49.00	1767.0
50.00	7618.0
51.00	2567.0
51.90	120.0
53.10	129.0
55.10	147.0
55.90	542.0
57.00	1131.0
60.10	363.0
61.00	2259.0
62.00	2040.0
63.00	1932.0
64.00	372.0
65.00	360.0
66.80	133.0
68.10	4384.0
69.00	4321.0
70.10	400.0
72.20	242.0
73.00	1748.0
74.00	7080.0
75.00	20248.0
76.00	1973.0
77.00	200.0
78.00	246.0
78.90	1861.0
79.90	521.0
81.00	1843.0
81.90	489.0
87.00	1555.0
87.90	1772.0
91.00	159.0
92.00	1399.0
93.00	2154.0
94.00	4800.0
95.00	38784.0
96.00	2357.0
103.80	198.0
106.00	276.0
115.90	168.0
116.90	397.0
118.00	300.0
118.90	330.0
129.90	164.0
134.90	105.0
136.80	135.0
140.90	432.0
142.90	682.0
145.00	331.0
147.80	104.0
170.90	130.0
172.10	470.0
173.10	469.0
174.00	33224.0
175.00	2631.0
176.00	32096.0
177.00	1834.0

Instrument :
MSVOA_V
ClientSampleId :
BFB281

m/z	Abundance
36.00	463.0
37.00	1761.0
38.00	1663.0
39.00	766.0
39.90	310.0
44.00	590.0
45.00	381.0
47.10	392.0
47.90	308.0
49.00	1444.0
50.00	7009.0
51.00	2397.0
51.90	153.0
53.10	102.0
55.10	150.0
55.90	541.0
57.00	1053.0
60.00	292.0
61.00	2141.0
62.00	1834.0
63.00	1688.0
64.00	355.0
65.00	439.0
68.10	4102.0
69.00	4041.0
70.10	401.0
72.10	242.0
73.00	1596.0
74.00	6636.0
75.00	18776.0
76.00	1904.0
77.00	199.0
77.90	250.0
78.90	1783.0
79.90	536.0
80.90	1795.0
81.90	435.0
87.00	1470.0
87.90	1668.0
91.00	152.0
92.00	1196.0
93.00	2143.0
94.00	4445.0
95.00	36264.0
96.00	2087.0
103.80	186.0
106.00	321.0
116.00	151.0
116.90	381.0
118.00	243.0
118.90	304.0
127.80	110.0
129.90	156.0
136.80	158.0
141.10	405.0
142.90	582.0
145.00	300.0
156.70	115.0
171.00	100.0
172.10	466.0
173.10	472.0
174.00	31352.0
175.00	2408.0
176.00	30000.0
177.00	1951.0

Instrument :
MSVOA_V
ClientSampleId :
BFB281