
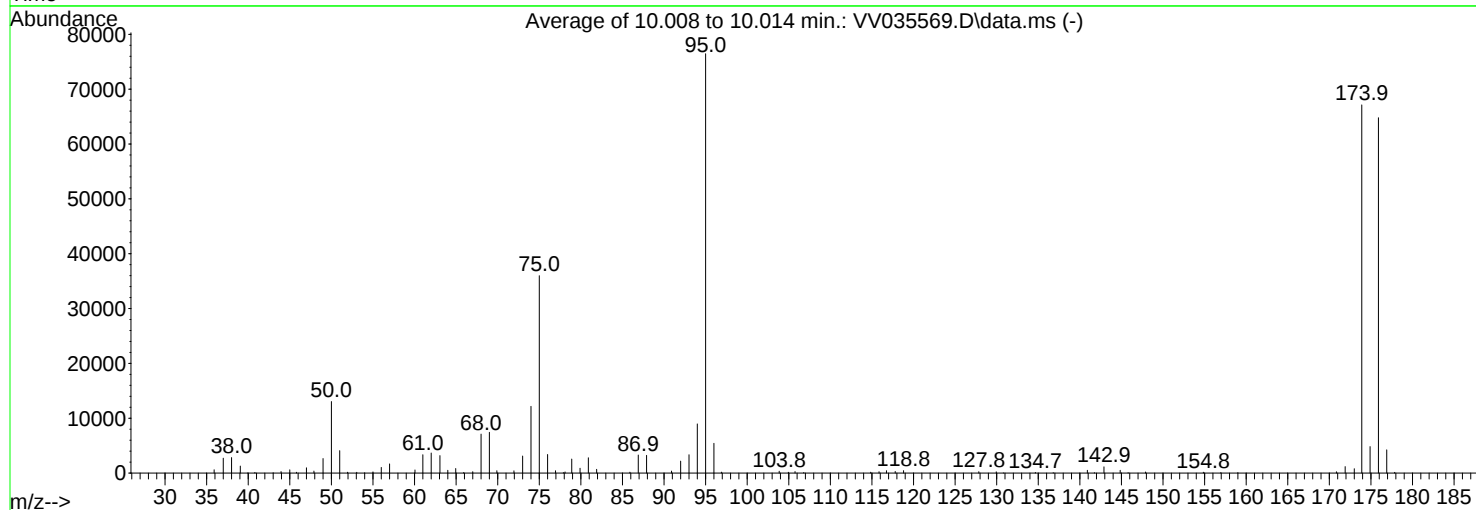


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051024\
Data File : VV035569.D
Acq On : 10 May 2024 08:43
Operator : SY/MD
Sample : BFB301
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB301

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM050124WMA.M
Title : VOC Analysis
Last Update : Fri May 10 23:44:12 2024

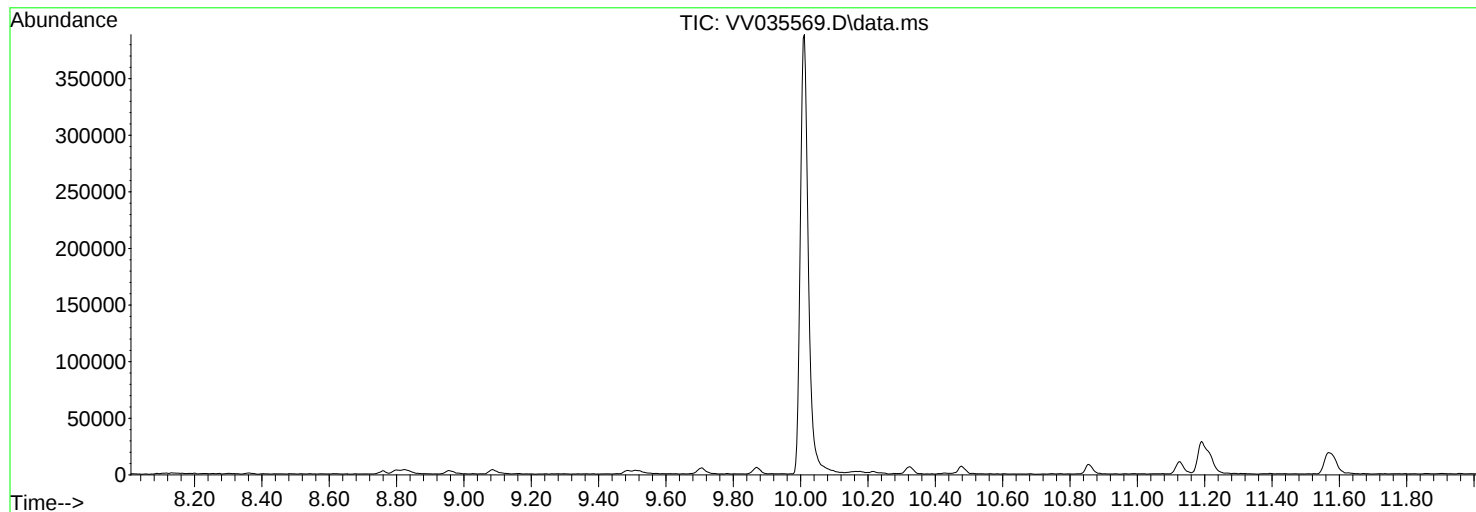

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	13040	PASS
75	95	30	80	47.1	35992	PASS
95	95	100	100	100.0	76467	PASS
96	95	5	9	7.1	5428	PASS
173	174	0.00	2	1.2	797	PASS
174	95	50	120	87.8	67139	PASS
175	174	5	9	7.2	4836	PASS
176	174	95	105	96.5	64797	PASS
177	176	5	10	6.5	4241	PASS

Scan 2778 (9.972 min): VV035569.D\data.ms
BFB301

m/z	Abundance
39.90	306.0
43.90	575.0
77.10	134.0

Instrument :
MSVOA_V
ClientSampleId :
BFB301

m/z	Abundance
35.90	634.0
37.00	2804.0
38.00	2888.0
39.10	1347.0
39.90	337.0
40.80	118.0
43.00	102.0
44.00	882.0
45.00	645.0
45.80	153.0
47.00	913.0
47.90	363.0
49.00	2780.0
50.00	13715.0
51.00	4419.0
51.90	173.0
53.10	167.0
55.00	232.0
56.00	1154.0
57.00	1820.0
60.00	610.0
61.00	3413.0
62.00	3681.0
63.00	3495.0
64.00	590.0
64.90	899.0
65.90	137.0
67.00	275.0
68.00	7144.0
69.00	7727.0
69.90	492.0
71.90	411.0
73.00	3172.0
74.00	12478.0
75.00	37136.0
76.00	3515.0
76.90	577.0
77.90	266.0
78.90	2734.0
79.90	904.0
80.90	2699.0
81.90	679.0
85.90	178.0
86.90	3242.0
87.90	3201.0
90.90	349.0
92.00	2143.0
93.00	3264.0
94.00	9291.0
95.00	78728.0
96.00	5539.0
96.90	175.0
103.80	366.0
105.00	123.0
105.80	301.0
106.80	111.0
114.90	156.0
115.80	275.0
116.80	449.0
117.80	295.0
118.80	469.0
127.90	243.0
130.00	228.0
130.80	101.0
134.60	125.0
136.80	123.0
140.90	517.0
142.90	1237.0
144.80	564.0
145.80	125.0
147.90	203.0
154.90	188.0
159.00	106.0
170.90	242.0
171.90	1148.0
173.00	756.0
173.90	67792.0
174.90	4774.0
175.90	65016.0
176.90	4483.0
177.90	135.0

Instrument :
MSVOA_V
ClientSampleId :
BFB301

m/z	Abundance
35.90	620.0
37.00	2834.0
38.00	2931.0
39.00	1298.0
39.90	318.0
40.80	136.0
44.00	851.0
45.00	607.0
45.80	170.0
47.00	958.0
47.90	396.0
49.00	2721.0
50.00	13513.0
51.00	4222.0
52.00	163.0
53.00	152.0
54.00	100.0
55.00	223.0
56.00	1067.0
57.00	1666.0
60.10	570.0
61.00	3479.0
62.00	3773.0
63.10	3218.0
64.00	512.0
65.00	843.0
65.90	116.0
67.00	266.0
68.00	7409.0
69.00	7626.0
69.90	420.0
72.00	433.0
73.00	3158.0
74.00	12547.0
75.00	36888.0
76.00	3467.0
76.90	575.0
78.10	297.0
78.90	2612.0
79.90	926.0
80.90	2879.0
81.90	696.0
85.90	178.0
86.90	3393.0
87.90	3340.0
90.90	401.0
92.00	2224.0
93.00	3403.0
94.00	9273.0
95.00	78920.0
96.00	5651.0
96.90	184.0
103.80	337.0
105.00	161.0
105.80	293.0
106.80	117.0
114.90	165.0
115.90	259.0
116.70	447.0
117.80	333.0
118.80	447.0
127.90	255.0
130.00	250.0
134.70	123.0
136.80	117.0
140.90	535.0
141.80	105.0
142.90	1185.0
144.80	504.0
145.80	105.0
147.90	209.0
154.90	168.0
157.00	119.0
159.00	105.0
170.80	247.0
171.90	1230.0
173.00	806.0
173.90	69200.0
174.90	5001.0
175.90	66960.0
176.90	4365.0
177.80	134.0

Instrument :
MSVOA_V
ClientSampleId :
BFB301

m/z	Abundance
35.90	563.0
37.00	2518.0
38.00	2652.0
39.00	1190.0
39.90	300.0
40.80	110.0
44.00	843.0
45.00	523.0
45.80	141.0
47.00	1009.0
47.90	358.0
49.00	2445.0
50.00	11891.0
51.00	3631.0
52.00	153.0
53.00	114.0
55.00	206.0
56.00	888.0
57.00	1523.0
60.10	526.0
61.00	3161.0
62.00	3532.0
63.10	2858.0
64.00	433.0
65.00	744.0
67.00	215.0
68.00	6767.0
69.00	6937.0
69.90	376.0
72.00	393.0
73.00	2992.0
74.00	11483.0
75.00	33952.0
76.00	3172.0
77.00	533.0
78.10	333.0
78.90	2334.0
79.90	829.0
80.90	2810.0
81.90	672.0
85.90	158.0
86.90	3229.0
87.90	3149.0
90.90	362.0
92.00	2188.0
93.00	3367.0
94.00	8320.0
95.00	71752.0
96.00	5094.0
96.90	164.0
103.90	323.0
104.90	162.0
105.70	268.0
106.80	104.0
114.80	158.0
115.90	232.0
116.70	413.0
117.80	280.0
118.80	421.0
127.80	258.0
129.90	251.0
134.70	106.0
140.90	474.0
141.70	117.0
142.90	994.0
144.90	448.0
147.90	196.0
154.80	126.0
156.90	123.0
170.80	254.0
171.90	1179.0
173.00	828.0
173.90	64424.0
174.90	4733.0
175.90	62416.0
176.90	3874.0
177.80	115.0

Instrument :
MSVOA_V
ClientSampleId :
BFB301