




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051124\
Data File : VV035578.D
Acq On : 10 May 2024 13:48
Operator : SY/MD
Sample : VSTD0.0507
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.05207

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 05/13/2024
Supervised By :Semsettin Yesilyurt 05/13/2024

Quant Time: May 11 01:01:31 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM051024.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat May 11 01:01:00 2024
Response via : Initial Calibration

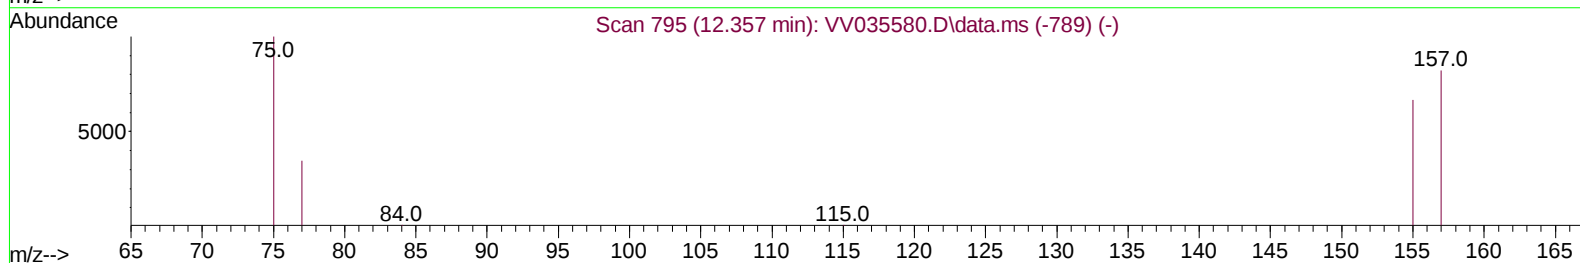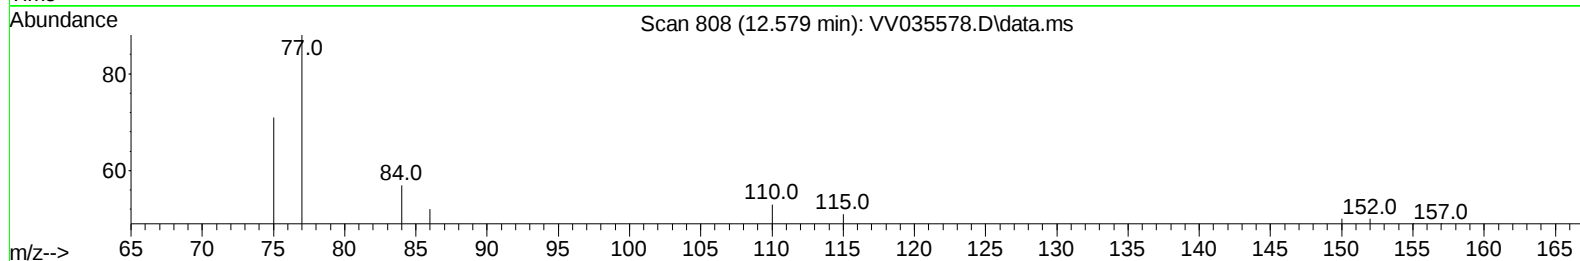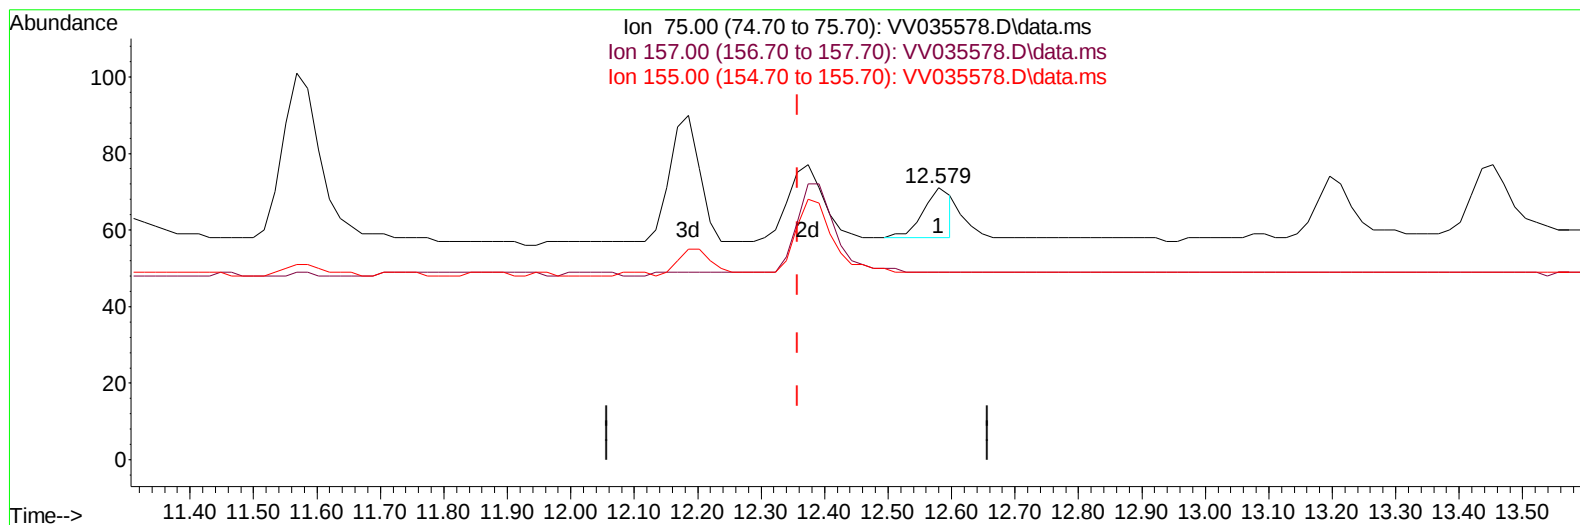

TIC: VV035578.D\data.ms

(13) 1,2-Dibromo-3-chloropropane (T)

12.579min (+ 0.222) 0.03 ug/L

response 40

Ion	Exp%	Act%
75.00	100.00	100.00
157.00	83.10	69.01
155.00	71.70	69.01
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051124\
 Data File : VV035578.D
 Acq On : 10 May 2024 13:48
 Operator : SY/MD
 Sample : VSTD0.0507
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.05207

Manual IntegrationsAPPROVED

Quant Time: May 11 01:01:31 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM051024.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat May 11 01:01:00 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 05/13/2024
 Supervised By :Semsettin Yesilyurt 05/13/2024

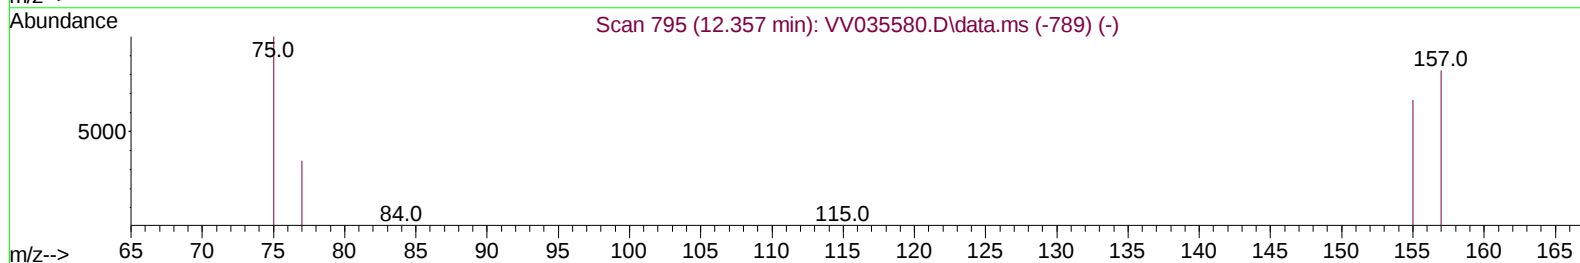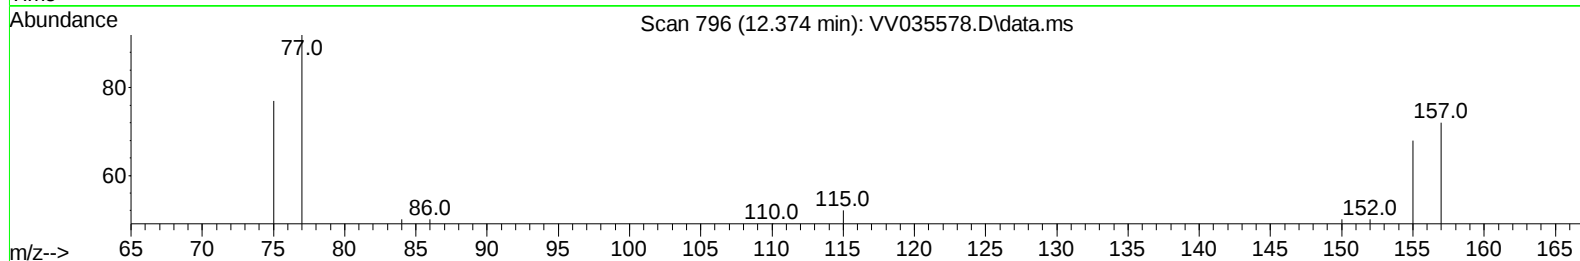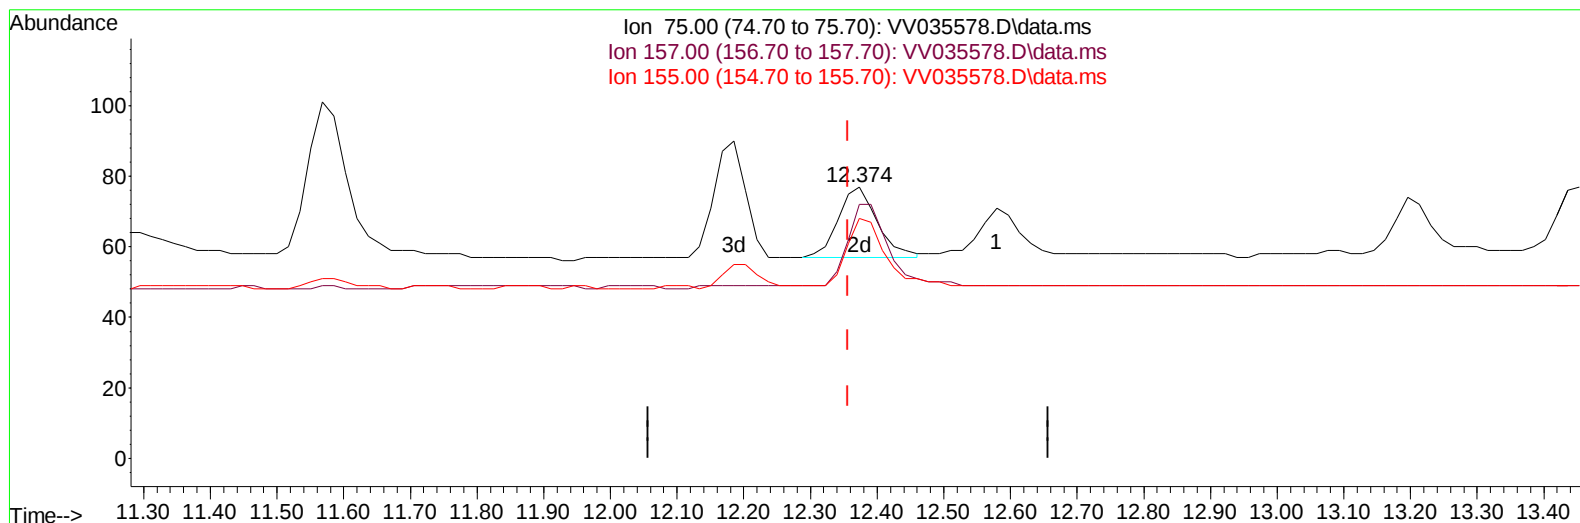

TIC: VV035578.D\data.ms

(13) 1,2-Dibromo-3-chloropropane (T)

12.374min (+ 0.017) 0.06 ug/L m

response 81

Ion	Exp%	Act%
75.00	100.00	100.00
157.00	83.10	93.51
155.00	71.70	88.31#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051124\
 Data File : VV035578.D
 Acq On : 10 May 2024 13:48
 Operator : SY/MD
 Sample : VSTD0.0507
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.05207

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 05/13/2024
 Supervised By :Semsettin Yesilyurt 05/13/2024

Quant Time: May 11 01:01:31 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM051024.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat May 11 01:01:00 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	10405	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	10494	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152	5760	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.273	65	367	0.052	ug/L	0.00
4) 1,2-Dichloroethane-d4	4.993	65	414	0.051	ug/L	0.02
7) 1,2-Dichloropropane-d6	6.019	67	440	0.048	ug/L	0.02
8) Toluene-d8	7.269	98	1208	0.052	ug/L	0.02
10) 1,1,2,2-Tetrachloroeth...	10.146	84	392	0.049	ug/L	0.00
Target Compounds						
						Qvalue
3) Vinyl chloride	1.280	62	577	0.059	ug/L	82
6) Trichloroethene	5.852	95	460	0.057	ug/L	92
9) 1,2-Dibromoethane	8.305	107	309	0.052	ug/L #	92
12) 1,2,3-Trichloropropane	10.214	75	330	0.055	ug/L	96
13) 1,2-Dibromo-3-chloropr...	12.374	75	81m	0.057	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051124\
Data File : VV035578.D
Acq On : 10 May 2024 13:48
Operator : SY/MD
Sample : VSTD0.0507
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.05207

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 05/13/2024
Supervised By :Semsettin Yesilyurt 05/13/2024

Quant Time: May 11 01:01:31 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM051024.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat May 11 01:01:00 2024
Response via : Initial Calibration

