




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051124\
Data File : VV035579.D
Acq On : 10 May 2024 14:12
Operator : SY/MD
Sample : VSTD0.108
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.1208

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 05/13/2024
Supervised By :Semsettin Yesilyurt 05/13/2024

Quant Time: May 11 01:01:42 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM051024.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat May 11 01:01:00 2024
Response via : Initial Calibration

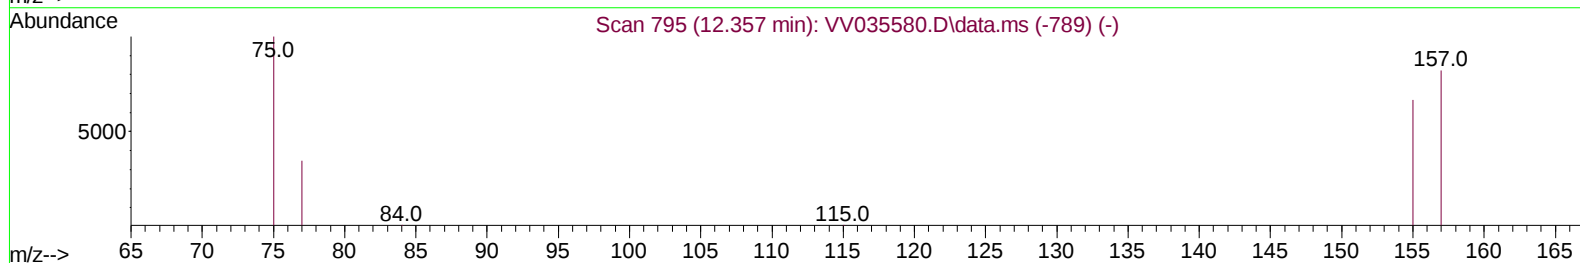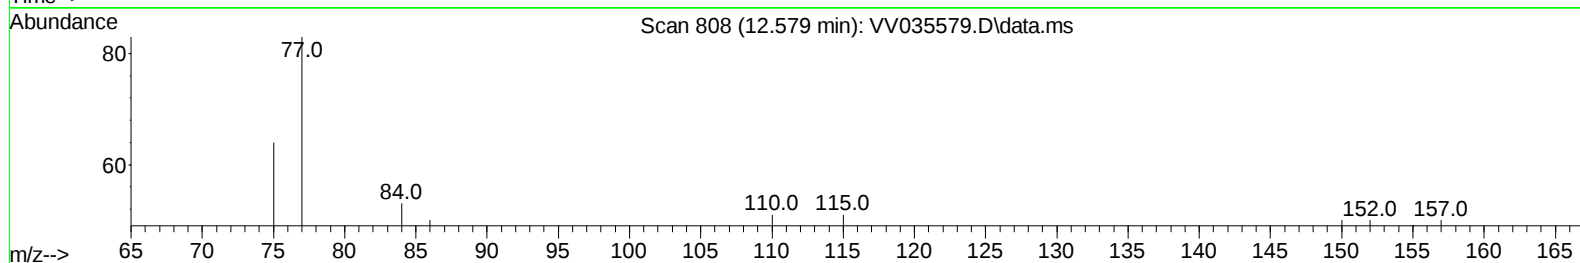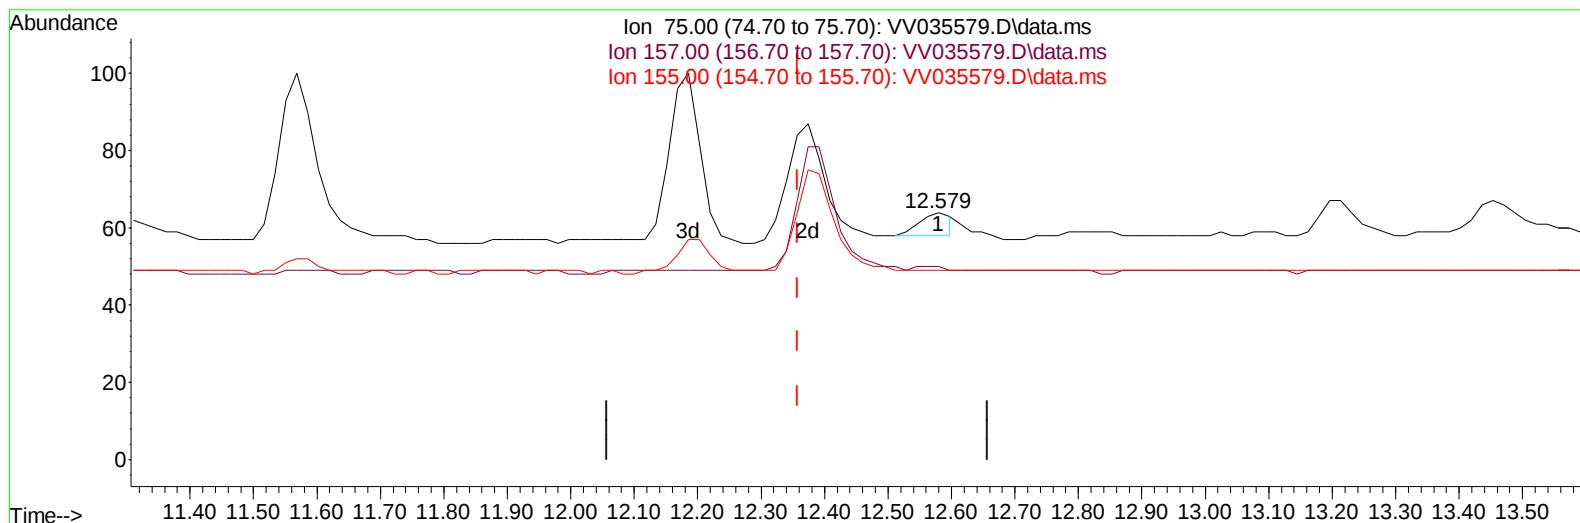

TIC: VV035579.D\data.ms

(13) 1,2-Dibromo-3-chloropropane (T)

12.579min (+ 0.222) 0.02 ug/L

response 21

Ion	Exp%	Act%
75.00	100.00	100.00
157.00	83.10	78.13
155.00	71.70	76.56
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051124\
 Data File : VV035579.D
 Acq On : 10 May 2024 14:12
 Operator : SY/MD
 Sample : VSTD0.108
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.1208

Manual IntegrationsAPPROVED

Quant Time: May 11 01:01:42 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM051024.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat May 11 01:01:00 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 05/13/2024
 Supervised By :Semsettin Yesilyurt 05/13/2024

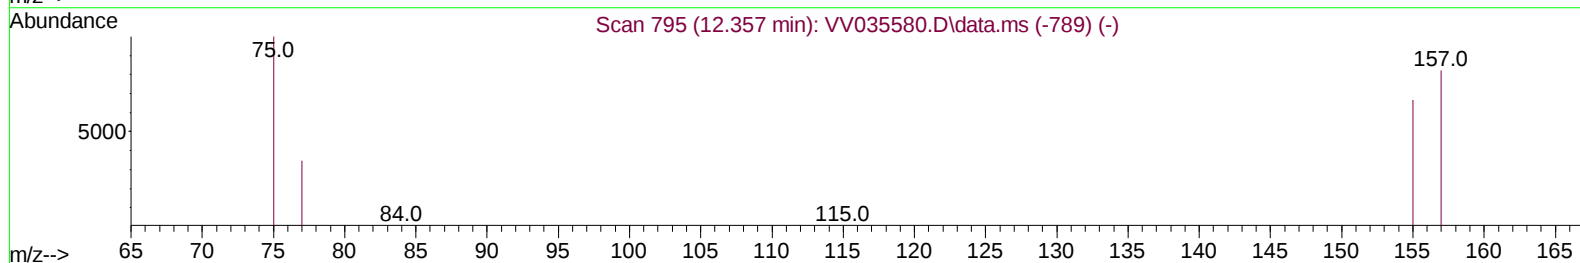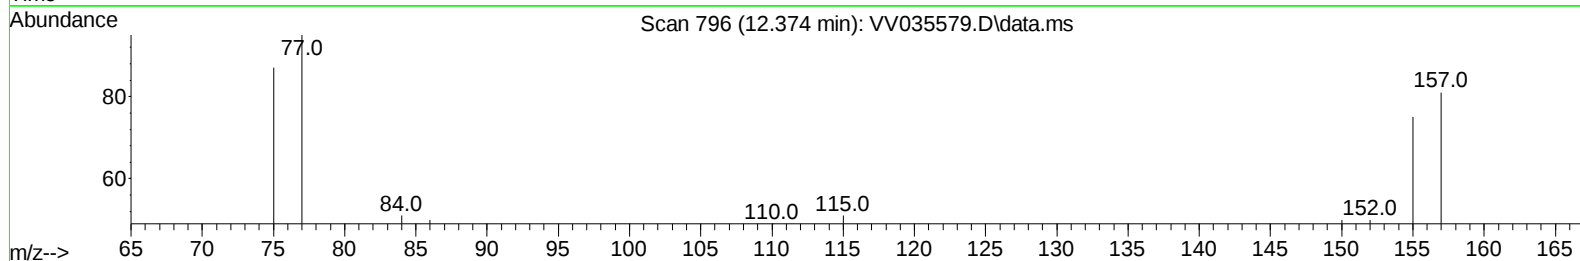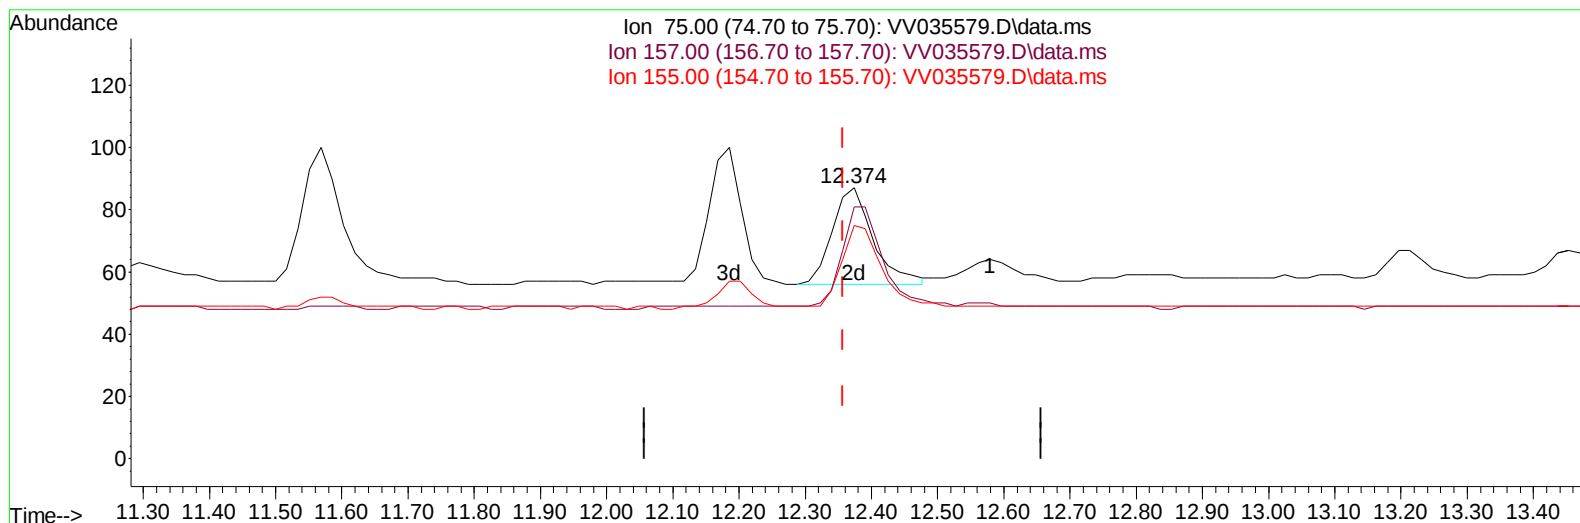

TIC: VV035579.D\data.ms

(13) 1,2-Dibromo-3-chloropropane (T)

12.374min (+ 0.017) 0.10 ug/L m

response 134

Ion	Exp%	Act%
75.00	100.00	100.00
157.00	83.10	93.10
155.00	71.70	86.21#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051124\
 Data File : VV035579.D
 Acq On : 10 May 2024 14:12
 Operator : SY/MD
 Sample : VSTD0.108
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.1208

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 05/13/2024
 Supervised By :Semsettin Yesilyurt 05/13/2024

Quant Time: May 11 01:01:42 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM051024.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat May 11 01:01:00 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	9846	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	9903	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152	5526	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	715	0.106	ug/L	0.00
4) 1,2-Dichloroethane-d4	4.993	65	763	0.099	ug/L	0.02
7) 1,2-Dichloropropane-d6	6.019	67	875	0.101	ug/L	0.02
8) Toluene-d8	7.269	98	2230	0.101	ug/L	0.02
10) 1,1,2,2-Tetrachloroeth...	10.146	84	760	0.102	ug/L	0.00
Target Compounds						
						Qvalue
3) Vinyl chloride	1.280	62	926	0.100	ug/L	90
6) Trichloroethene	5.852	95	706	0.093	ug/L	95
9) 1,2-Dibromoethane	8.305	107	543	0.097	ug/L #	92
12) 1,2,3-Trichloropropane	10.214	75	519	0.091	ug/L	97
13) 1,2-Dibromo-3-chloropr...	12.374	75	134m	0.098	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051124\
Data File : VV035579.D
Acq On : 10 May 2024 14:12
Operator : SY/MD
Sample : VSTD0.108
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.1208

Manual IntegrationsAPPROVED

Quant Time: May 11 01:01:42 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM051024.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat May 11 01:01:00 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 05/13/2024
Supervised By :Semsettin Yesilyurt 05/13/2024

