
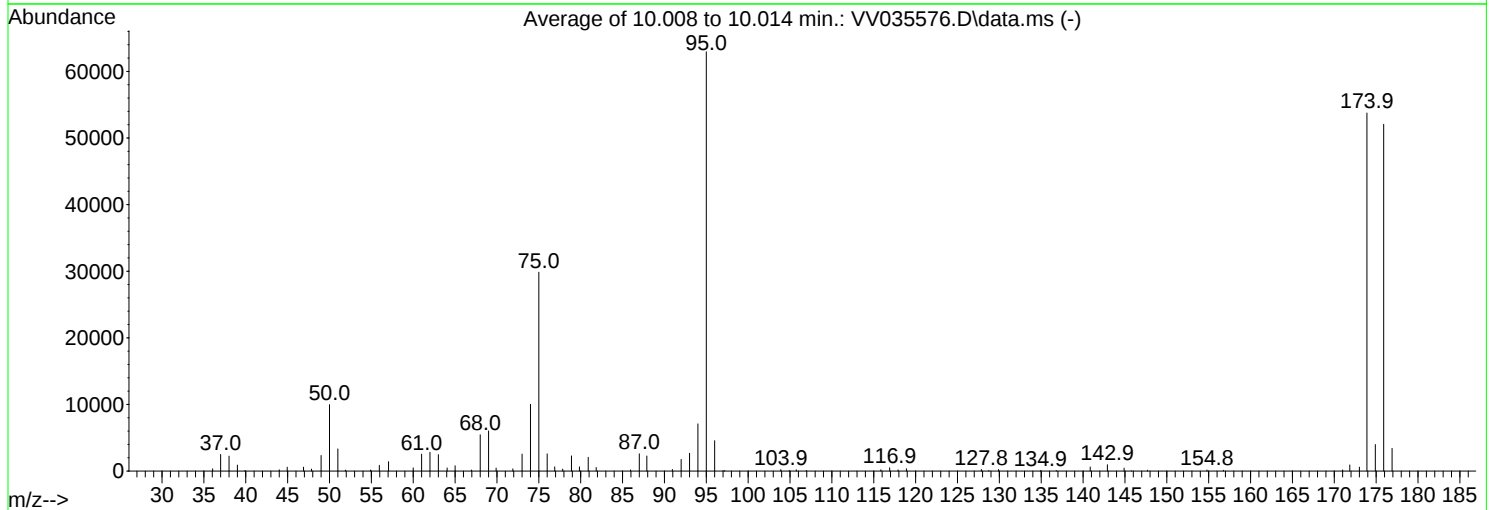


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051124\
Data File : VV035576.D
Acq On : 10 May 2024 12:36
Operator : SY/MD
Sample : BFB205
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB205

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM051024.M
Title : TRACE VOA SOM01.0
Last Update : Sat May 11 01:09:31 2024

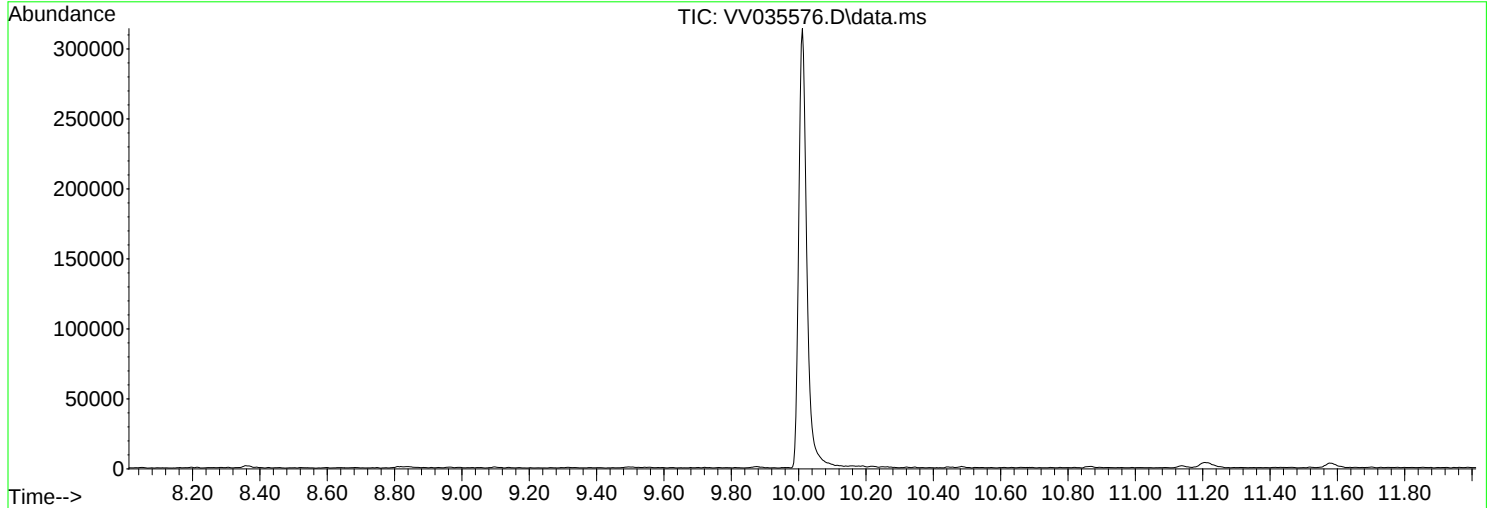

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.8	9977	PASS
75	95	30	80	47.4	29845	PASS
95	95	100	100	100.0	62952	PASS
96	95	5	9	7.2	4560	PASS
173	174	0.00	2	1.1	592	PASS
174	95	50	120	85.4	53763	PASS
175	174	5	9	7.4	3987	PASS
176	174	95	101	96.8	52067	PASS
177	176	5	9	6.6	3415	PASS

m/z	Abundance
39.90	236.0
44.00	653.0

Instrument :
MSVOA_V
ClientSampleId :
BFB205

m/z	Abundance
36.00	347.0
37.00	2495.0
38.00	2340.0
39.00	902.0
40.00	296.0
44.00	779.0
45.00	604.0
46.90	576.0
47.90	334.0
49.00	2436.0
50.00	10224.0
51.00	3309.0
51.90	144.0
54.90	202.0
56.00	830.0
57.00	1383.0
60.00	487.0
61.00	2699.0
62.00	2969.0
63.00	2514.0
64.00	464.0
65.00	738.0
66.90	155.0
68.00	5403.0
69.00	6139.0
69.90	497.0
71.90	341.0
73.00	2478.0
74.00	10246.0
75.00	30352.0
76.00	2780.0
76.90	602.0
77.80	328.0
78.90	2230.0
79.80	604.0
80.90	2034.0
81.80	514.0
86.00	104.0
87.00	2613.0
87.90	2364.0
91.00	265.0
92.00	1730.0
93.00	2745.0
94.00	7241.0
95.00	62408.0
96.00	4640.0
97.00	115.0
103.90	236.0
105.70	183.0
115.80	205.0
116.90	468.0
117.90	184.0
118.90	367.0
127.80	228.0
129.90	237.0
134.90	147.0
136.80	120.0
140.90	598.0
142.90	920.0
144.90	421.0
145.80	119.0
147.70	139.0
154.80	155.0
156.70	112.0
171.00	185.0
171.90	963.0
173.00	536.0
173.90	52584.0
174.90	4013.0
175.90	50768.0
176.90	3300.0

Instrument :
MSVOA_V
ClientSampleId :
BFB205

m/z	Abundance
36.10	333.0
37.00	2578.0
38.00	2355.0
39.00	908.0
39.90	295.0
44.00	848.0
45.00	601.0
46.90	608.0
47.90	288.0
49.00	2415.0
50.00	10211.0
51.00	3426.0
51.90	157.0
54.90	166.0
55.90	885.0
57.10	1430.0
60.00	497.0
61.00	2590.0
62.00	2904.0
63.00	2532.0
64.10	479.0
65.00	848.0
66.90	160.0
68.00	5644.0
69.00	6237.0
69.90	468.0
71.90	356.0
73.00	2608.0
74.00	10270.0
75.00	30752.0
76.00	2660.0
76.90	677.0
77.80	306.0
78.90	2341.0
79.90	632.0
80.90	2125.0
81.90	535.0
85.90	188.0
87.00	2667.0
87.90	2322.0
91.00	258.0
92.00	1804.0
93.00	2779.0
94.00	7248.0
95.00	65088.0
96.00	4737.0
97.20	108.0
103.90	230.0
104.90	113.0
105.80	205.0
106.90	113.0
115.80	204.0
116.90	488.0
117.90	192.0
119.00	353.0
127.90	254.0
128.80	101.0
129.90	248.0
134.90	121.0
136.80	117.0
140.90	642.0
142.90	1014.0
144.90	478.0
147.70	152.0
154.80	167.0
156.80	126.0
171.00	181.0
171.80	950.0
173.00	621.0
173.90	55616.0
174.90	4088.0
175.90	53864.0
176.90	3546.0

Instrument :
MSVOA_V
ClientSampleId :
BFB205

m/z	Abundance
36.00	356.0
37.00	2410.0
38.00	2059.0
39.00	896.0
39.90	312.0
44.00	913.0
44.90	568.0
46.90	591.0
47.80	265.0
49.00	2176.0
50.00	9495.0
51.00	3267.0
51.90	153.0
54.80	111.0
56.00	879.0
57.00	1426.0
60.00	470.0
61.00	2352.0
62.00	2607.0
63.00	2379.0
64.10	482.0
65.00	824.0
67.00	171.0
68.00	5308.0
69.00	5720.0
69.90	384.0
71.90	331.0
73.00	2584.0
74.00	9571.0
75.00	28432.0
76.00	2334.0
76.90	618.0
77.90	266.0
78.90	2287.0
79.80	667.0
80.90	2024.0
81.90	583.0
85.90	233.0
87.00	2506.0
87.90	2114.0
90.90	218.0
92.00	1721.0
93.00	2500.0
94.00	6778.0
95.00	61360.0
96.00	4302.0
97.20	127.0
103.90	208.0
104.90	114.0
105.80	227.0
107.00	104.0
115.90	208.0
116.90	537.0
117.90	173.0
118.80	341.0
127.90	262.0
128.70	126.0
129.90	232.0
140.80	626.0
142.90	918.0
144.90	448.0
147.70	132.0
154.80	188.0
156.80	133.0
171.00	152.0
171.80	860.0
173.00	618.0
173.90	53088.0
174.90	3861.0
175.90	51568.0
176.90	3400.0

Instrument :
MSVOA_V
ClientSampleId :
BFB205