

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV051419\
Quantitation Report (QT Reviewed)


Data File : VV010898.D
Acq On : 15 May 2019 13:28
Operator : SY/MD
Sample : K2788-11
Misc : 5.98G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A51A0

Manual Integrations
APPROVED

MMDadoda
5/20/2019 1:04:19 AM

Quant Time: May 16 08:01:43 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM051319S.M
Quant Title : VOC Analysis
QLast Update : Thu May 16 07:25:32 2019
Response via : Initial Calibration

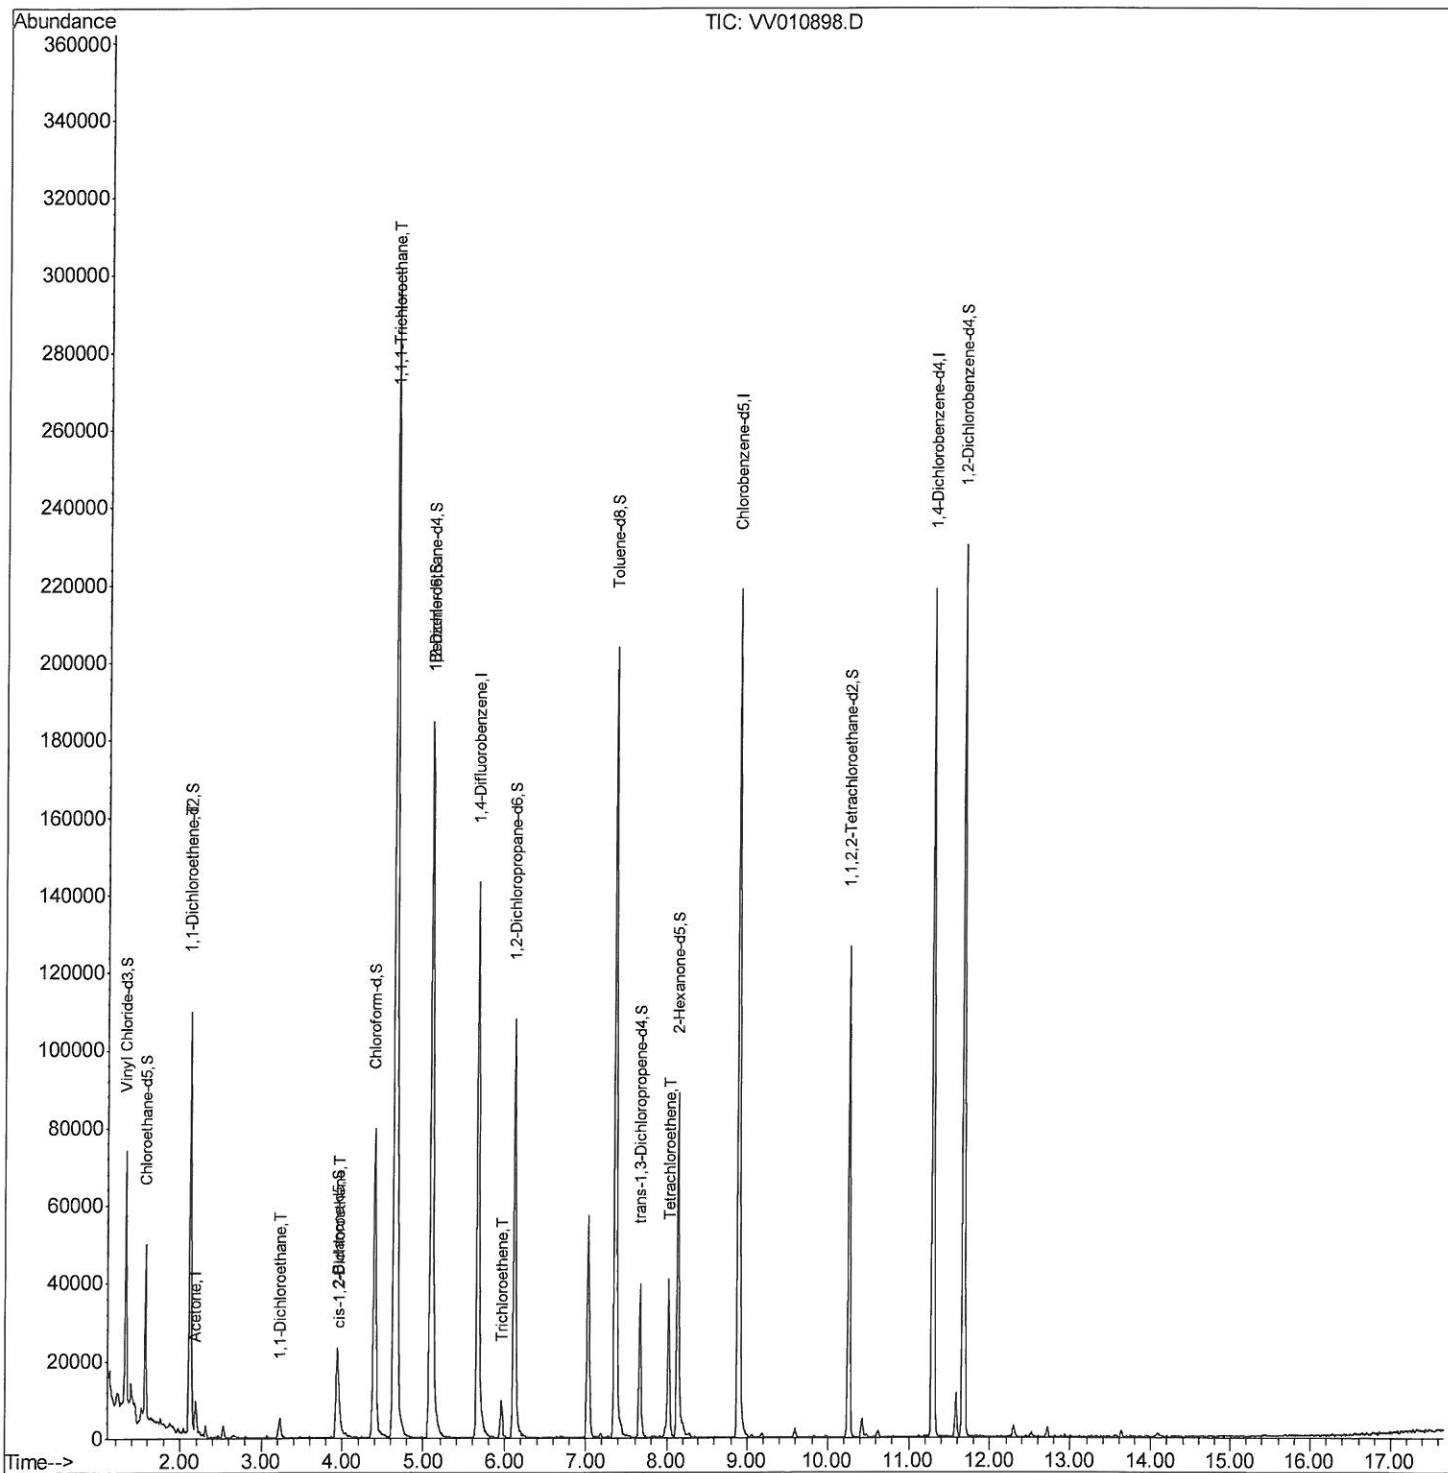

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV051419\
Quantitation Report (Qedit)




Data File : VV010898.D
Acq On : 15 May 2019 13:28
Operator : SY/MD
Sample : K2788-11
Misc : 5.98G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A51A0

Manual Integrations
APPROVED

MMDadoda
5/20/2019 1:04:19 AM

Quant Time: May 16 07:29:20 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM051319S.M
Quant Title : VOC Analysis
QLast Update : Thu May 16 07:25:32 2019
Response via : Initial Calibration

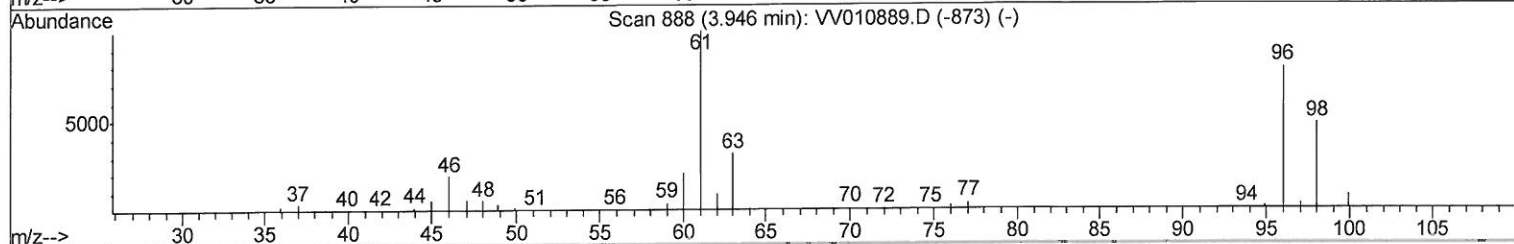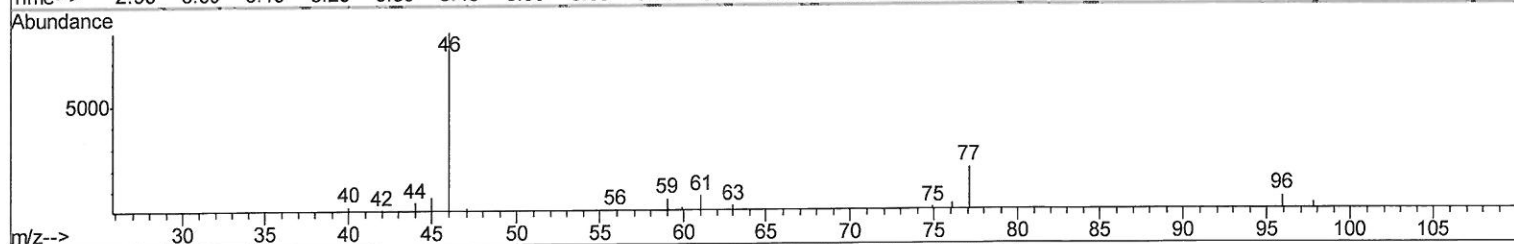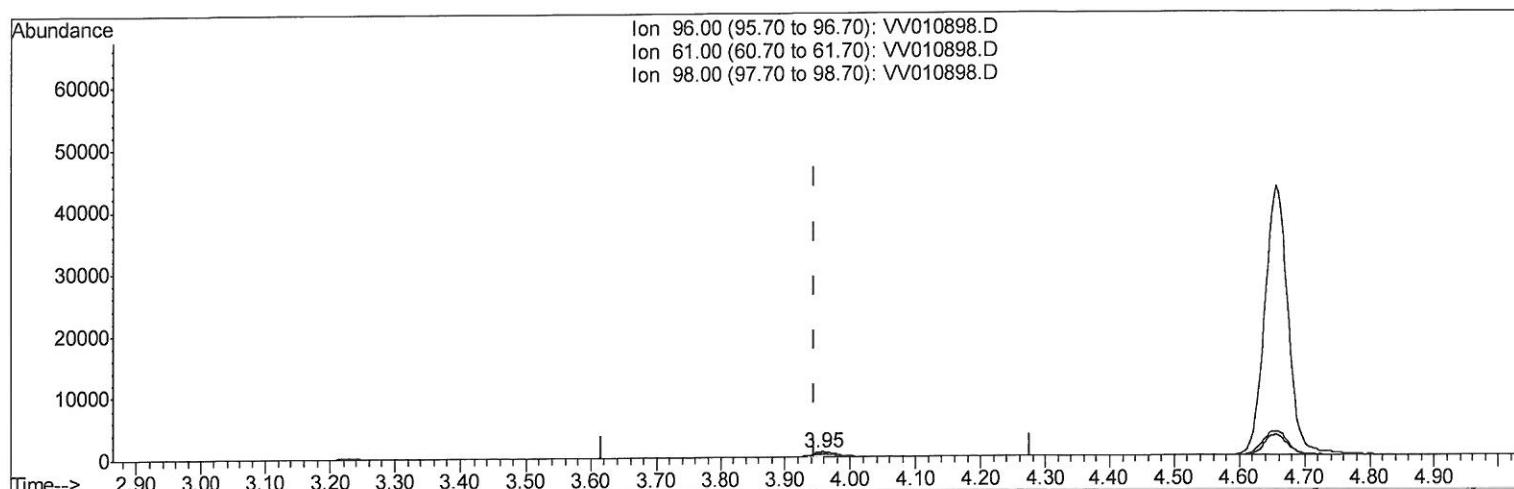

TIC: VV010898.D

(22) cis-1,2-Dichloroethene (T)

3.952min (+0.006) 0.39ug/L

response 774

Ion	Exp%	Act%
96.00	100	100
61.00	128.90	115.04
98.00	63.10	56.34
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV051419\
Quantitation Report (Qedit)




Data File : VV010898.D
Acq On : 15 May 2019 13:28
Operator : SY/MD
Sample : K2788-11
Misc : 5.98G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A51A0

Manual Integrations
APPROVED

MMDadoda
5/20/2019 1:04:19 AM

Quant Time: May 16 07:29:20 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM051319S.M
Quant Title : VOC Analysis
QLast Update : Thu May 16 07:25:32 2019
Response via : Initial Calibration

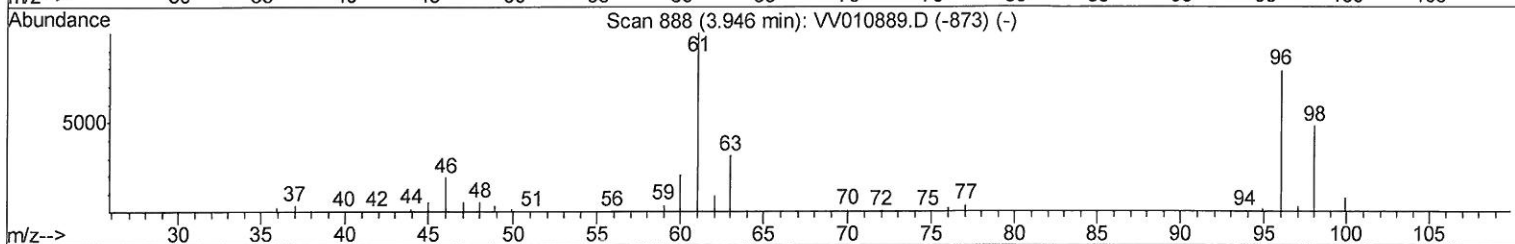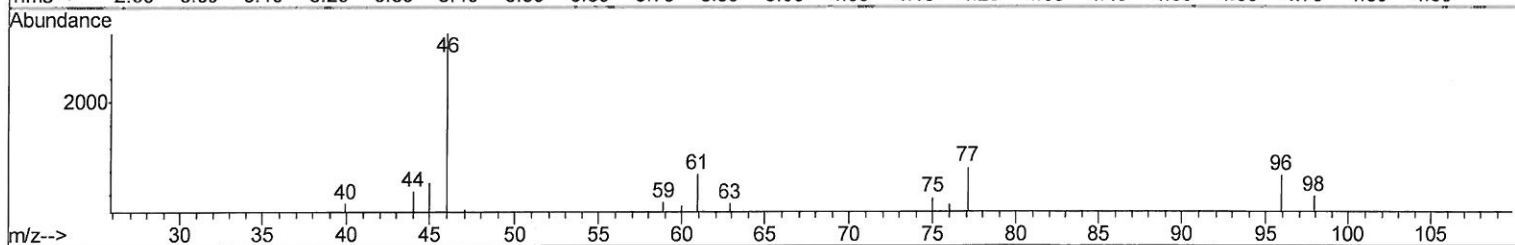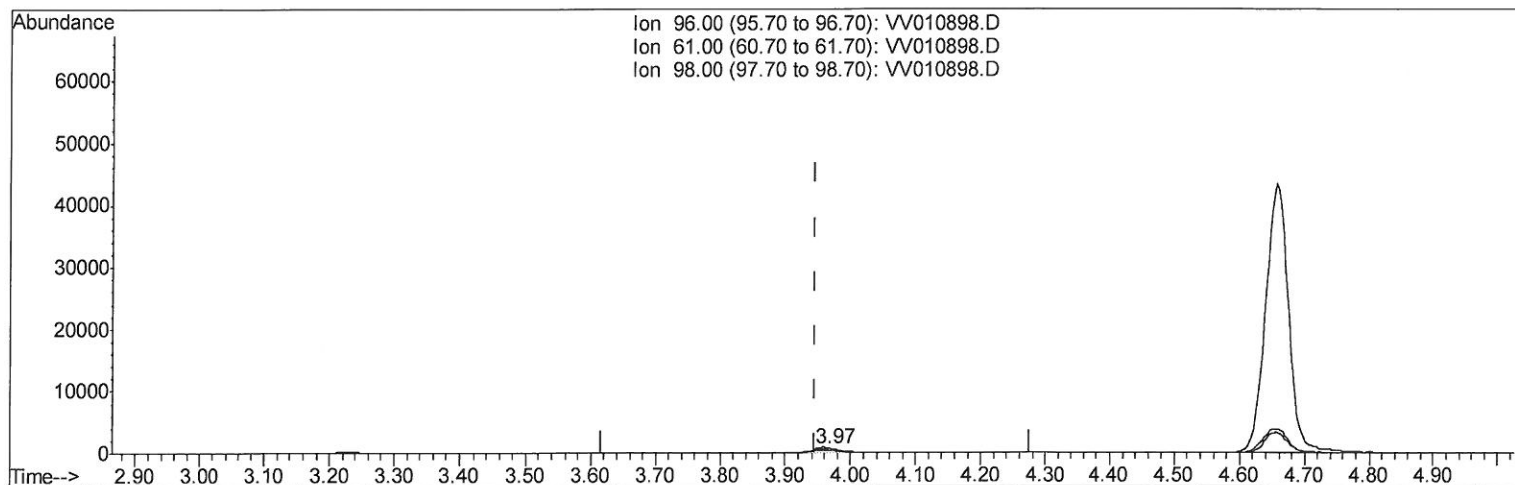

TIC: VV010898.D

(22) cis-1,2-Dichloroethene (T)

3.968min (+0.022) 0.94ug/L m

response 1859

Ion	Exp%	Act%
96.00	100	100
61.00	128.90	102.61
98.00	63.10	51.10
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV051419\
 Quantitation Report (QT Reviewed)
 Data File : VV010898.D
 Acq On : 15 May 2019 13:28
 Operator : SY/MD
 Sample : K2788-11
 Misc : 5.98G/10ML/MSVOA_V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A51A0

Manual Integrations
 APPROVED

MMDadoda
 5/20/2019 1:04:19 AM

Quant Time: May 16 08:01:43 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM051319S.M
 Quant Title : VOC Analysis
 QLast Update : Thu May 16 07:25:32 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	122826	25.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	129483	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	57383	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	34922	22.32	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.28%
7) Chloroethane-d5	1.57	69	26662	26.14	ug/L	0.02
Spiked Amount	25.000	Range	30 - 150	Recovery	=	104.56%
10) 1,1-Dichloroethene-d2	2.13	63	53699	18.13	ug/L	0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	72.52%
20) 2-Butanone-d5	3.93	46	35575	72.26	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	144.52%#
24) Chloroform-d	4.40	84	82333	23.22	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	92.88%
26) 1,2-Dichloroethane-d4	5.08	65	51497	25.54	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	102.16%
29) Benzene-d6	5.10	84	160788	22.43	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	89.72%
33) 1,2-Dichloropropane-d6	6.12	67	54575	23.87	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	95.48%
37) Toluene-d8	7.36	98	147002	21.34	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	85.36%
38) trans-1,3-Dichloropropene-	7.66	79	21512	21.57	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	86.28%
39) 2-Hexanone-d5	8.13	63	29473	68.02	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	136.04%#
48) 1,1,2,2-Tetrachloroethane-	10.26	84	60765	28.65	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	114.60%
61) 1,2-Dichlorobenzene-d4	11.67	152	59807	24.95	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	99.80%

Target Compounds

					Qvalue	
12) 1,1-Dichloroethene	2.14	96	2236	1.580	ug/L	# 1
13) Acetone	2.19	43	6444	12.850	ug/L	92
19) 1,1-Dichloroethane	3.23	63	5143	1.576	ug/L	# 94
22) cis-1,2-Dichloroethene	3.97	96	1859m	0.942	ug/L	98
31) 1,1,1-Trichloroethane	4.66	97	244136	86.811	ug/L	98
35) Trichloroethene	5.96	95	3194	1.633	ug/L	94
47) Tetrachloroethene	8.02	164	9153	6.333	ug/L	97

05/20/19 Sy

(#) = qualifier out of range (m) = manual integration (+) = signals summed