

Data File : VV010879.D
Acq On : 15 May 2019 01:05
Operator : SY/MD
Sample : K2798-07
Misc : 4.55G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DB877

Quant Time: May 15 08:26:30 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM051319S.M
Quant Title : VOC Analysis
QLast Update : Wed May 15 08:08:35 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	135935	25.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	127038	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	47887	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	37452	21.63	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	86.52%
7) Chloroethane-d5	1.56	69	29177	25.85	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	103.40%
10) 1,1-Dichloroethene-d2	2.12	63	56426	17.22	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	68.88%
20) 2-Butanone-d5	3.93	46	20944	38.44	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	76.88%
24) Chloroform-d	4.39	84	76623	19.52	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	78.08%
26) 1,2-Dichloroethane-d4	5.07	65	51637	23.14	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	92.56%
29) Benzene-d6	5.09	84	172912	24.59	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	98.36%
33) 1,2-Dichloropropane-d6	6.11	67	56533	25.20	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	100.80%
37) Toluene-d8	7.36	98	149081	22.06	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	88.24%
38) trans-1,3-Dichloropropene-	7.66	79	19383	19.81	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	79.24%
39) 2-Hexanone-d5	8.13	63	13913	32.73	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	65.46%
48) 1,1,2,2-Tetrachloroethane-	10.26	84	48594	23.36	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	93.44%
61) 1,2-Dichlorobenzene-d4	11.67	152	46046	23.02	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	92.08%


Target Compounds					Qvalue
13) Acetone	2.18	43	8723	15.717 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VV010879.D
Acq On : 15 May 2019 01:05
Operator : SY/MD
Sample : K2798-07
Misc : 4.55G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DB877

Quant Time: May 15 08:26:30 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM051319S.M
Quant Title : VOC Analysis
QLast Update : Wed May 15 08:08:35 2019
Response via : Initial Calibration

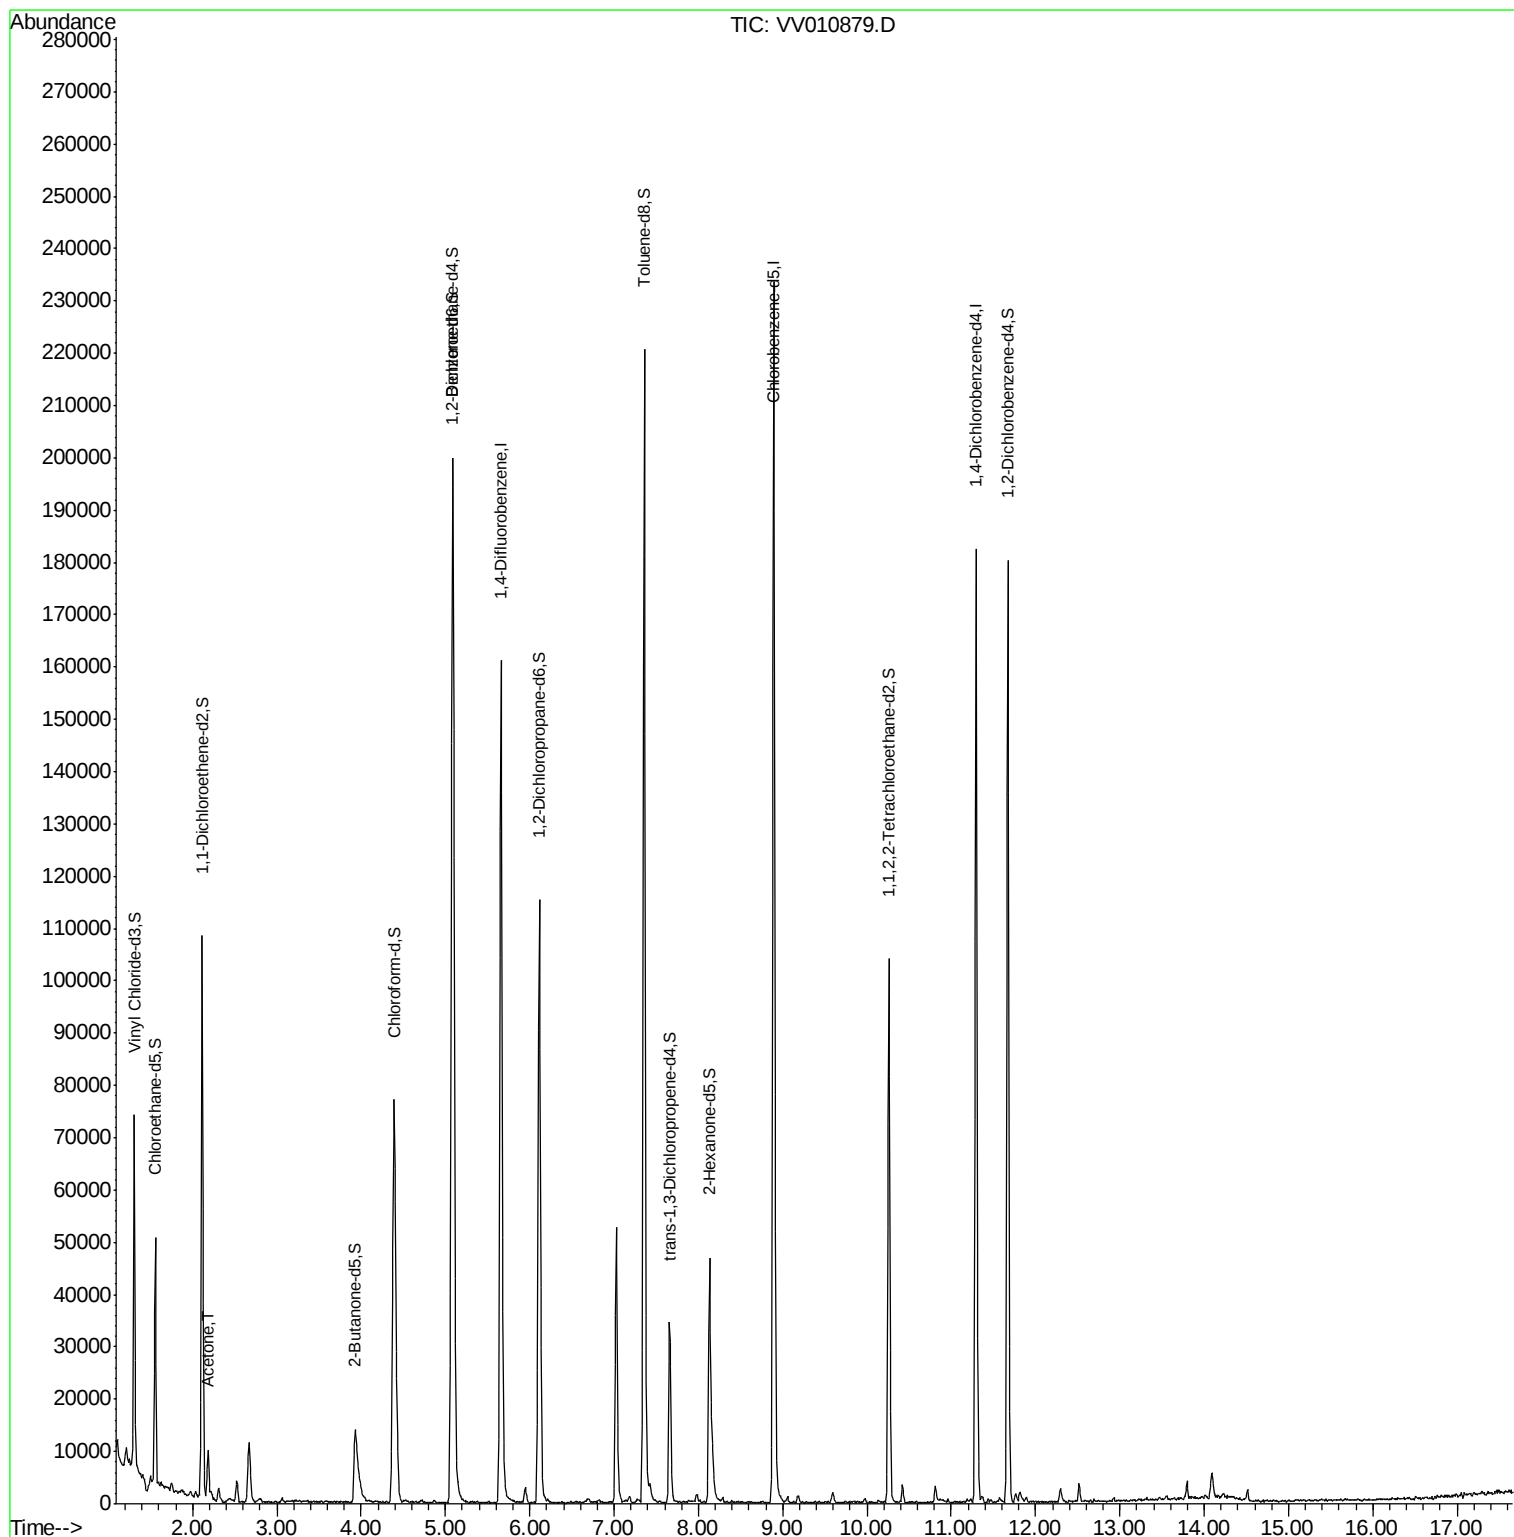

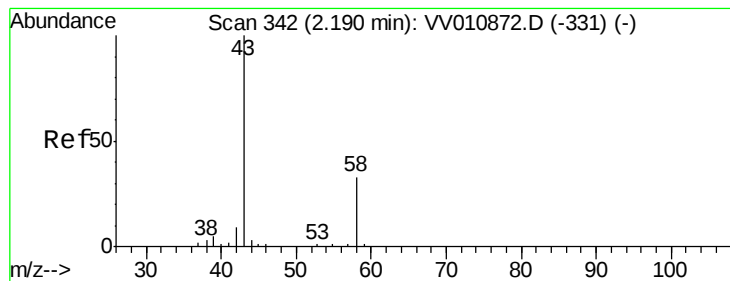

#13
Acetone
Concen: 15.717 ug/L
RT: 2.18 min Scan# 340
Delta R.T. -0.01 min
Lab File: VV010879.D
Acq: 15 May 2019 01:05

Instrument :
MSVOA_V
ClientSampleId :
DB877

Tgt Ion: 43 Resp: 8723
Ion Ratio Lower Upper
43 100
58 36.3 0.0 69.2

