

Data File : VV010888.D
Acq On : 15 May 2019 05:14
Operator : SY/MD
Sample : K2814-01
Misc : 5.07G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4246

Quant Time: May 15 08:58:43 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM051319S.M
Quant Title : VOC Analysis
QLast Update : Wed May 15 08:08:35 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	111917	25.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	96593	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	30427	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	32030	22.46	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.84%
7) Chloroethane-d5	1.57	69	27712	29.82	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	119.28%
10) 1,1-Dichloroethene-d2	2.12	63	46909	17.39	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	69.56%
20) 2-Butanone-d5	3.94	46	7387	16.47	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	32.94%
24) Chloroform-d	4.39	84	70086	21.69	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	86.76%
26) 1,2-Dichloroethane-d4	5.07	65	42346	23.05	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	92.20%
29) Benzene-d6	5.09	84	151809	28.39	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	113.56%
33) 1,2-Dichloropropane-d6	6.11	67	51280	30.06	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	120.24%#
37) Toluene-d8	7.36	98	121848	23.72	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	94.88%
38) trans-1,3-Dichloropropene-	7.66	79	13054	17.54	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	70.16%
39) 2-Hexanone-d5	8.13	63	7785	24.09	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	48.18%
48) 1,1,2,2-Tetrachloroethane-	10.26	84	34024	21.51	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	86.04%
61) 1,2-Dichlorobenzene-d4	11.67	152	31739	24.97	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	99.88%


Target Compounds					Qvalue
13) Acetone	2.18	43	190517	416.952 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VV010888.D
Acq On : 15 May 2019 05:14
Operator : SY/MD
Sample : K2814-01
Misc : 5.07G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4246

Quant Time: May 15 08:58:43 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM051319S.M
Quant Title : VOC Analysis
QLast Update : Wed May 15 08:08:35 2019
Response via : Initial Calibration

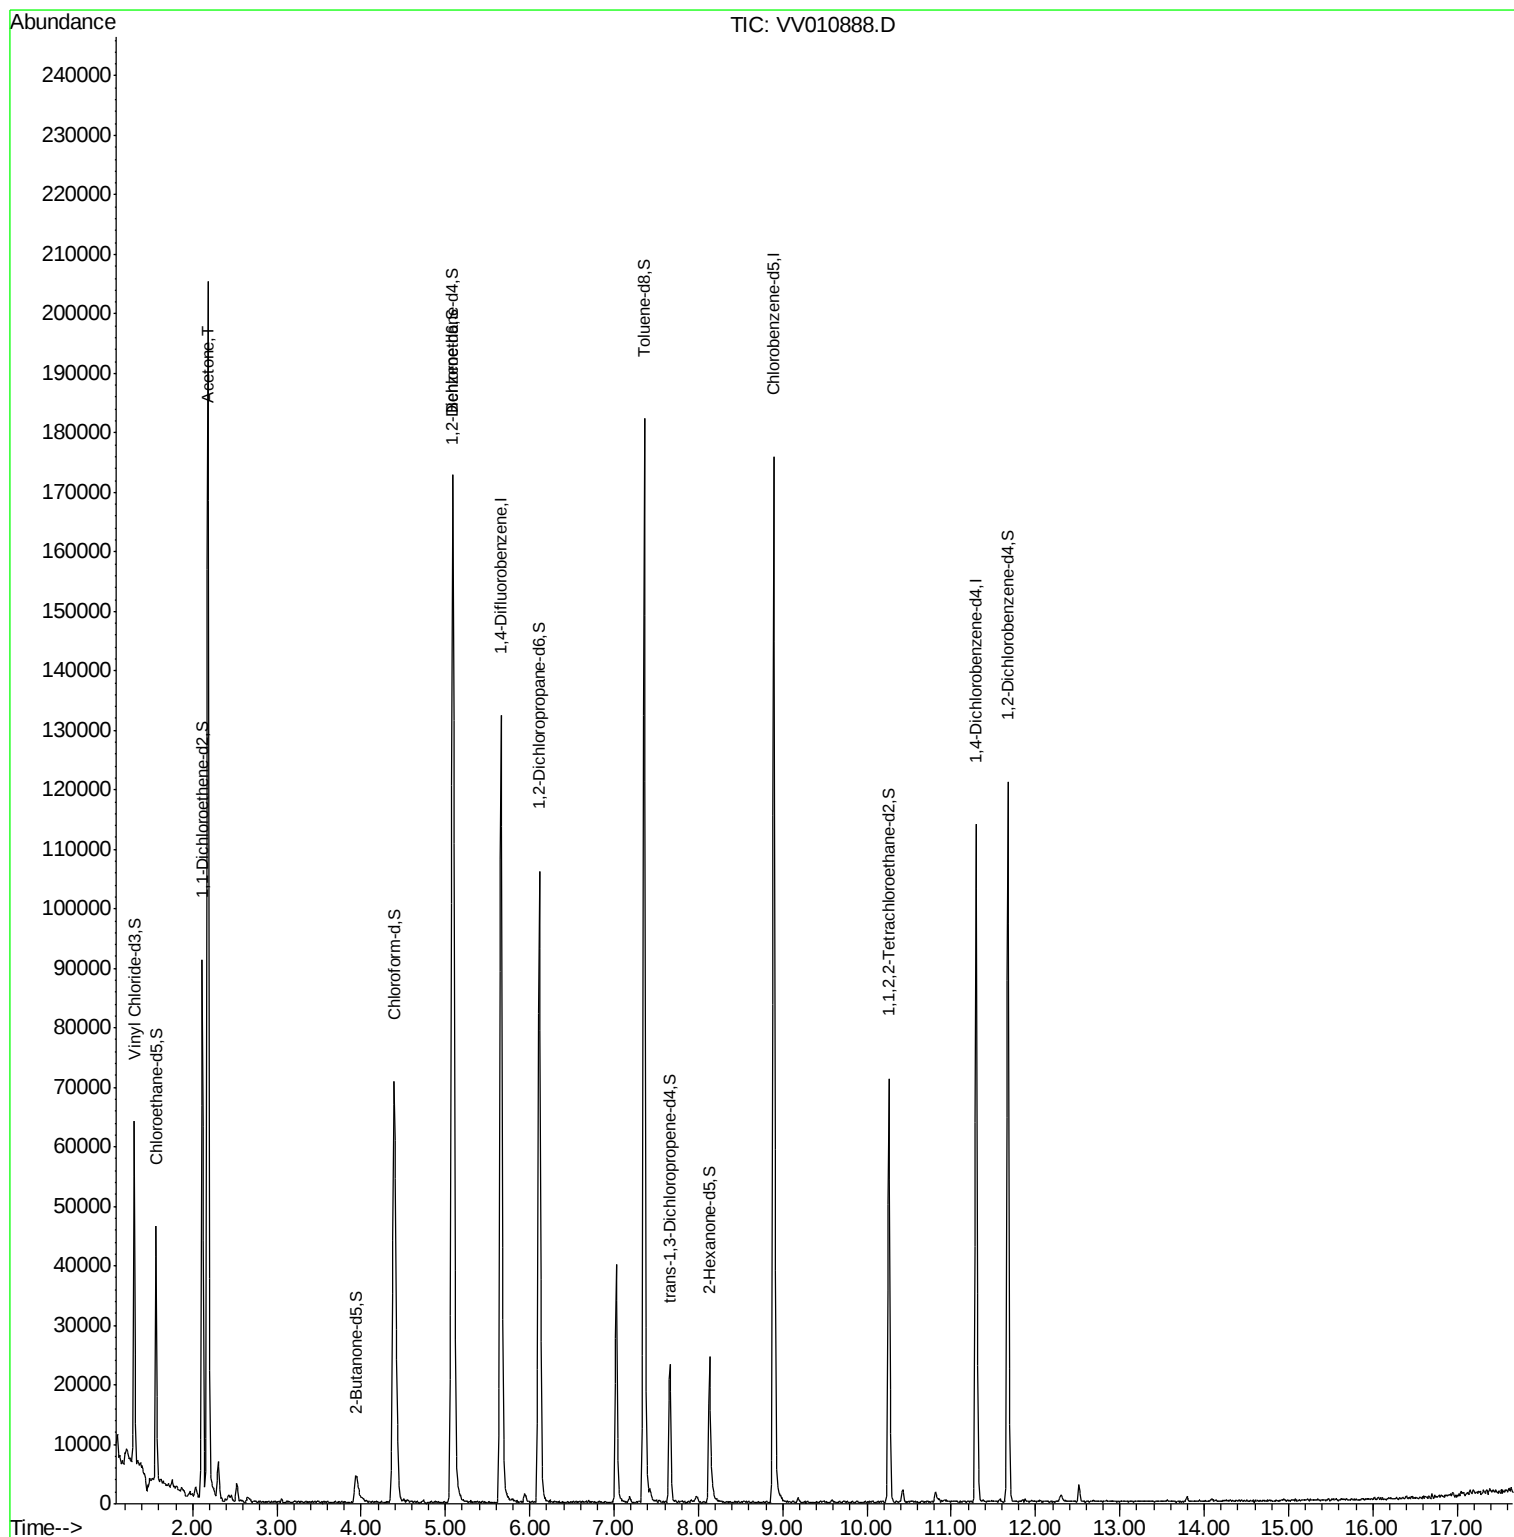

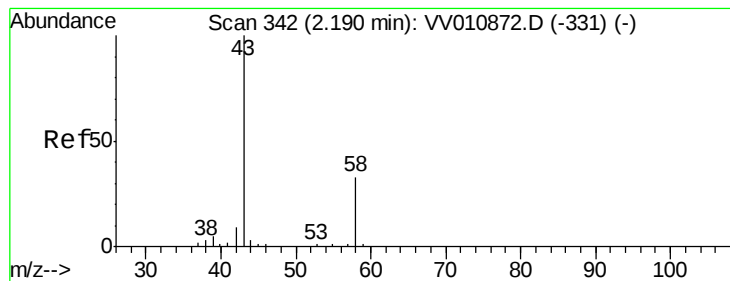

#13
 Acetone
 Concen: 416.952 ug/L
 RT: 2.18 min Scan# 339
 Delta R.T. -0.01 min
 Lab File: VV010888.D
 Acq: 15 May 2019 05:14

Instrument :
 MSVOA_V
 ClientSampleId :
 A4246

Tgt Ion: 43 Resp: 190517
 Ion Ratio Lower Upper
 43 100
 58 32.4 0.0 69.2

