

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV051419\
 Data File : VV010905.D
 Acq On : 15 May 2019 19:56
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.00G/10ML/MSVOA_V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM051319S.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	65	70	77	rVB	70725	65838	13.75%	1.912%
2	1.563	141	147	157	rVB	47133	54588	11.40%	1.585%
3	2.122	311	321	333	rBV	116008	162616	33.96%	4.721%
4	2.531	441	448	458	rVB3	2471	3948	0.82%	0.115%
5	3.071	608	616	620	rVB5	494	689	0.14%	0.020%
6	3.161	641	644	646	rBV2	227	156	0.03%	0.005%
7	3.180	646	650	653	rVV2	164	173	0.04%	0.005%
8	3.466	735	739	742	rBV2	194	200	0.04%	0.006%
9	3.817	845	848	849	rBV	165	113	0.02%	0.003%
10	3.881	867	868	870	rBV	110	58	0.01%	0.002%
11	3.936	874	885	910	rBV	17234	46288	9.67%	1.344%
12	4.216	967	972	977	rBV2	221	362	0.08%	0.011%
13	4.238	977	979	980	rBV	70	32	0.01%	0.001%
14	4.245	980	981	986	rBV	106	91	0.02%	0.003%
15	4.264	986	987	988	rBV	122	32	0.01%	0.001%
16	4.290	993	995	999	rVB	243	155	0.03%	0.005%
17	4.318	999	1004	1008	rBV2	247	223	0.05%	0.006%
18	4.399	1012	1029	1053	rBV2	73273	191761	40.05%	5.567%
19	4.563	1077	1080	1088	rBV3	324	476	0.10%	0.014%
20	4.756	1139	1140	1141	rBV	121	30	0.01%	0.001%
21	4.952	1197	1201	1205	rVB2	165	189	0.04%	0.005%
22	4.974	1205	1208	1210	rBV	199	134	0.03%	0.004%
23	5.003	1214	1217	1218	rBV	90	47	0.01%	0.001%
24	5.023	1218	1223	1224	rBV2	172	160	0.03%	0.005%
25	5.090	1228	1244	1284	rVV2	192293	478840	100.00%	13.902%
26	5.338	1319	1321	1326	rBV2	188	116	0.02%	0.003%
27	5.437	1349	1352	1353	rBV	64	38	0.01%	0.001%
28	5.447	1353	1355	1356	rVB	79	30	0.01%	0.001%
29	5.460	1357	1359	1361	rBV2	96	49	0.01%	0.001%
30	5.588	1394	1399	1404	rBV	261	293	0.06%	0.009%
31	5.662	1407	1422	1450	rBV2	141986	296609	61.94%	8.612%
32	5.884	1488	1491	1497	rVB	119	89	0.02%	0.003%
33	5.913	1497	1500	1501	rBV	128	76	0.02%	0.002%
34	5.923	1501	1503	1504	rBV	150	80	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV051419\
 Data File : VV010905.D
 Acq On : 15 May 2019 19:56
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.00G/10ML/MSVOA_V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM051319S.M
 Title : VOC Analysis

35	5.945	1504	1510	1513	rBV3	1002	1095	0.23%	0.032%
36	6.029	1534	1536	1539	rBV	165	125	0.03%	0.004%
37	6.055	1542	1544	1545	rBV	124	51	0.01%	0.001%
38	6.116	1546	1563	1594	rBV2	107953	222117	46.39%	6.449%
39	6.315	1622	1625	1627	rBV	186	100	0.02%	0.003%
40	6.328	1627	1629	1631	rVB	160	65	0.01%	0.002%
41	6.354	1635	1637	1641	rBV	142	143	0.03%	0.004%
42	6.424	1656	1659	1660	rBV	144	82	0.02%	0.002%
43	6.447	1663	1666	1668	rBV	167	136	0.03%	0.004%
44	6.482	1675	1677	1682	rBV2	184	198	0.04%	0.006%
45	6.537	1692	1694	1695	rBV	39	17	0.00%	0.000%
46	6.553	1695	1699	1700	rBV	154	130	0.03%	0.004%
47	6.585	1706	1709	1710	rBV	40	24	0.01%	0.001%
48	6.605	1710	1715	1720	rVB2	145	193	0.04%	0.006%
49	6.630	1720	1723	1725	rBV2	191	130	0.03%	0.004%
50	6.701	1738	1745	1748	rBV	830	922	0.19%	0.027%
51	6.733	1754	1755	1757	rVB	102	36	0.01%	0.001%
52	6.749	1757	1760	1766	rBV2	182	258	0.05%	0.007%
53	6.804	1774	1777	1779	rBV	261	191	0.04%	0.006%
54	6.913	1810	1811	1812	rBV	89	31	0.01%	0.001%
55	7.029	1832	1847	1866	rBV	55925	99891	20.86%	2.900%
56	7.148	1880	1884	1889	rVB2	274	284	0.06%	0.008%
57	7.183	1889	1895	1900	rBV2	338	479	0.10%	0.014%
58	7.241	1911	1913	1915	rVB	268	115	0.02%	0.003%
59	7.357	1937	1949	1986	rBV	215161	392614	81.99%	11.399%
60	7.576	2014	2017	2018	rBV	167	77	0.02%	0.002%
61	7.662	2034	2044	2061	rBV	38951	63507	13.26%	1.844%
62	7.820	2090	2093	2094	rBV2	106	60	0.01%	0.002%
63	7.868	2106	2108	2110	rVB2	171	57	0.01%	0.002%
64	7.913	2119	2122	2123	rBV2	189	87	0.02%	0.003%
65	7.981	2140	2143	2146	rBV3	555	323	0.07%	0.009%
66	8.026	2155	2157	2159	rBV	165	108	0.02%	0.003%
67	8.058	2164	2167	2170	rVB2	342	204	0.04%	0.006%
68	8.077	2170	2173	2176	rBV2	247	216	0.05%	0.006%
69	8.132	2180	2190	2208	rBV	59796	101426	21.18%	2.945%
70	8.312	2244	2246	2249	rBV	198	113	0.02%	0.003%
71	8.540	2313	2317	2322	rBV	243	316	0.07%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV051419\
 Data File : VV010905.D
 Acq On : 15 May 2019 19:56
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.00G/10ML/MSVOA_V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM051319S.M
 Title : VOC Analysis

72	8.894	2415	2427	2451	rBV	228202	379517	79.26%	11.019%
73	9.061	2473	2479	2480	rBV	481	499	0.10%	0.014%
74	9.450	2595	2600	2601	rBV	248	244	0.05%	0.007%
75	9.582	2639	2641	2642	rBB	105	90	0.02%	0.003%
76	9.961	2757	2759	2761	rBV	278	149	0.03%	0.004%
77	10.026	2777	2779	2782	rBV2	175	137	0.03%	0.004%
78	10.061	2789	2790	2793	rBV	107	71	0.01%	0.002%
79	10.100	2798	2802	2803	rBV	201	153	0.03%	0.004%
80	10.260	2841	2852	2870	rVB	106930	165519	34.57%	4.806%
81	10.424	2894	2903	2910	rBV4	2226	3477	0.73%	0.101%
82	10.823	3025	3027	3029	rVB2	314	114	0.02%	0.003%
83	10.881	3042	3045	3048	rBV	390	207	0.04%	0.006%
84	10.913	3052	3055	3056	rBV	297	124	0.03%	0.004%
85	10.958	3066	3069	3071	rBV3	533	257	0.05%	0.007%
86	10.993	3077	3080	3083	rBV2	260	135	0.03%	0.004%
87	11.190	3138	3141	3142	rBV2	389	247	0.05%	0.007%
88	11.296	3162	3174	3192	rBV	210846	344329	71.91%	9.997%
89	11.363	3193	3195	3197	rBV	388	180	0.04%	0.005%
90	11.672	3279	3291	3310	rBV	224012	349521	72.99%	10.148%
91	12.161	3439	3443	3448	rBV2	260	278	0.06%	0.008%
92	12.299	3477	3486	3497	rVB3	1975	3437	0.72%	0.100%
93	12.521	3550	3555	3561	rVB4	1235	1545	0.32%	0.045%
94	12.935	3680	3684	3685	rBV	197	155	0.03%	0.005%
95	13.058	3718	3722	3727	rBV	258	347	0.07%	0.010%
96	13.797	3944	3952	3958	rBV3	2195	2887	0.60%	0.084%
97	14.505	4169	4172	4174	rBV	305	186	0.04%	0.005%


Sum of corrected areas: 3444305

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV051419\
Data File : VV010905.D
Acq On : 15 May 2019 19:56
Operator : SY/MD
Sample : VIBLK
Misc : 5.00G/10ML/MSV0A_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VIBLK

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOM2VLM051319S.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

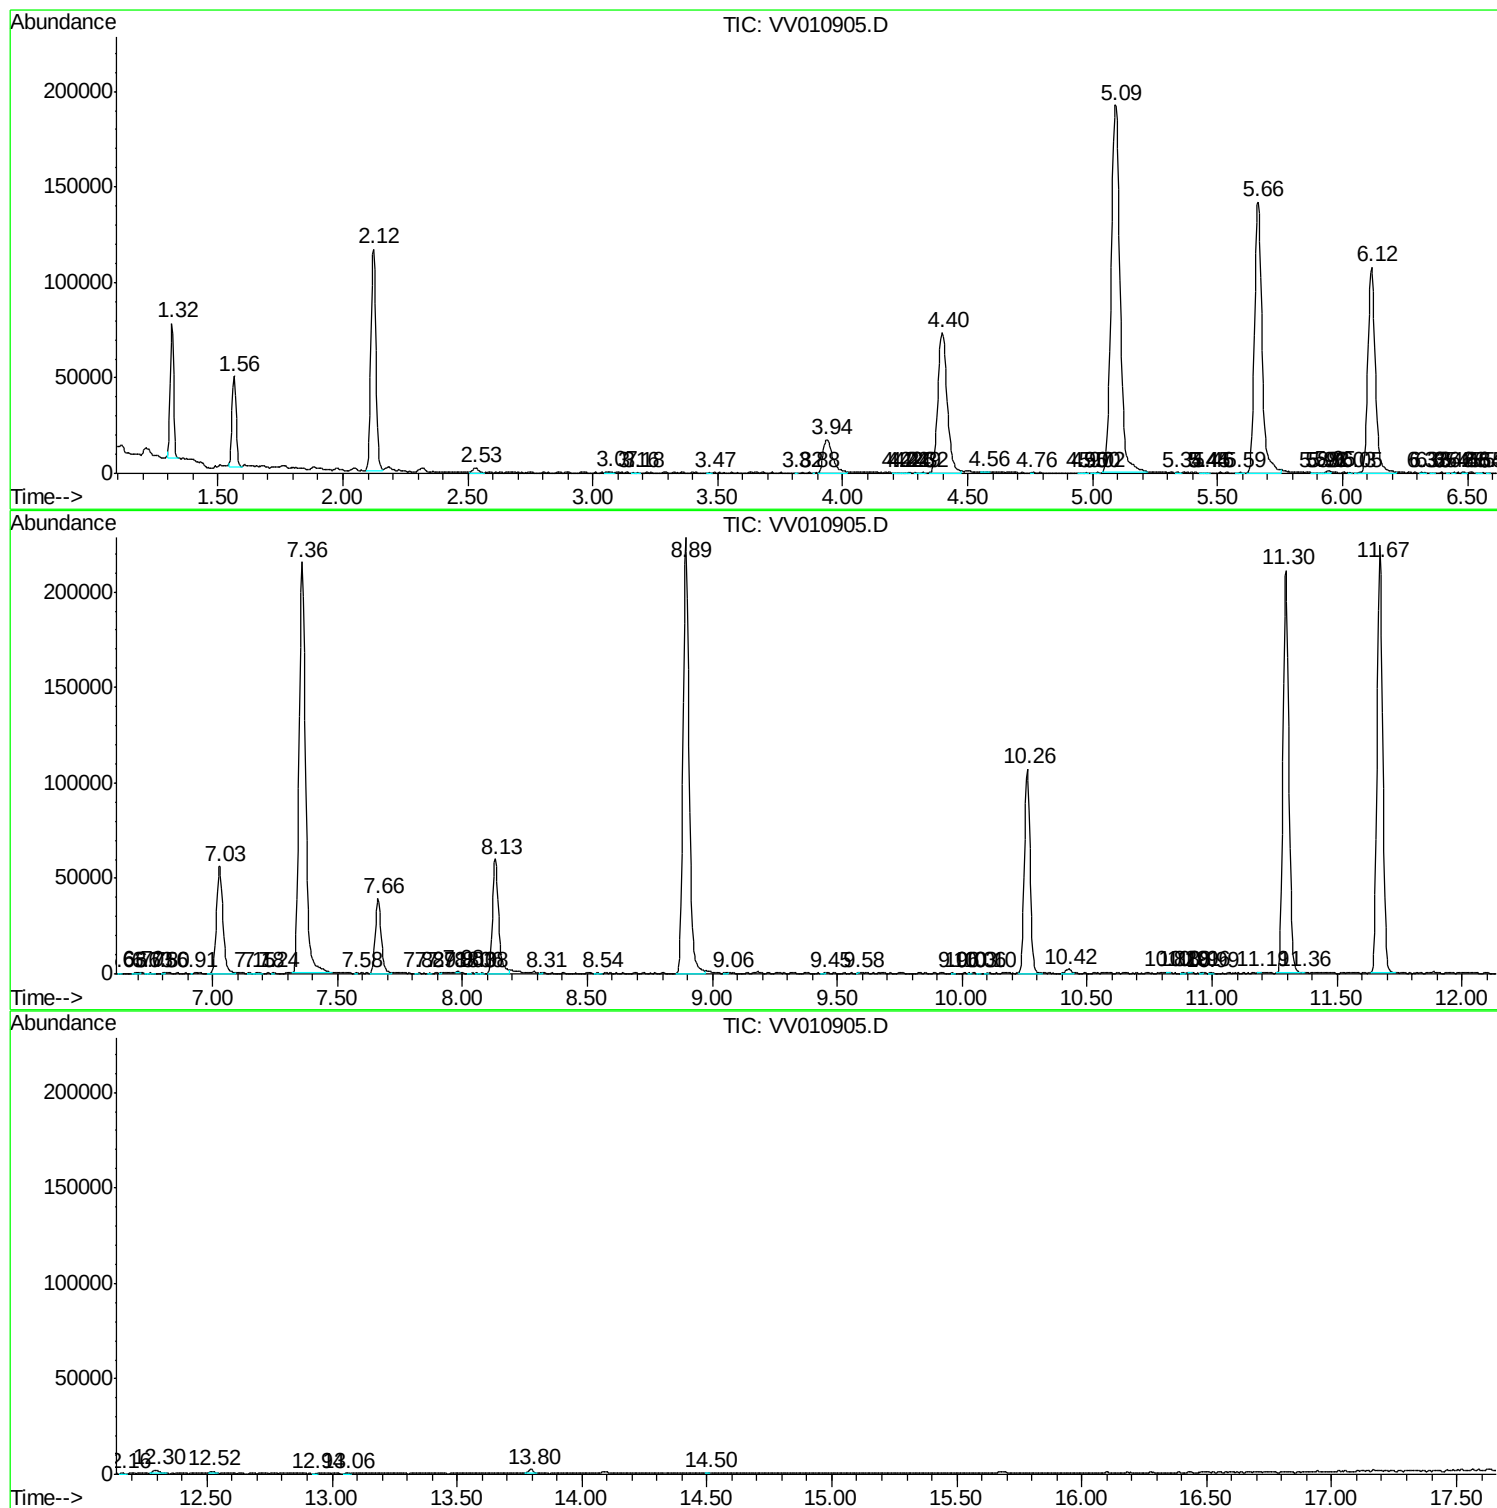

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV051419\
Data File : VV010905.D
Acq On : 15 May 2019 19:56
Operator : SY/MD
Sample : VIBLK
Misc : 5.00G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM051319S.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV051419\
Data File : VV010905.D
Acq On : 15 May 2019 19:56
Operator : SY/MD
Sample : VIBLK
Misc : 5.00G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM051319S.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc