


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV051419\
Data File : VV010852.D
Acq On : 14 May 2019 09:42
Operator : SY/MD
Sample : BFB97
Misc : 5.00G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB97

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM051319S.M
Title : VOC Analysis
Last Update : Mon May 20 01:26:07 2019

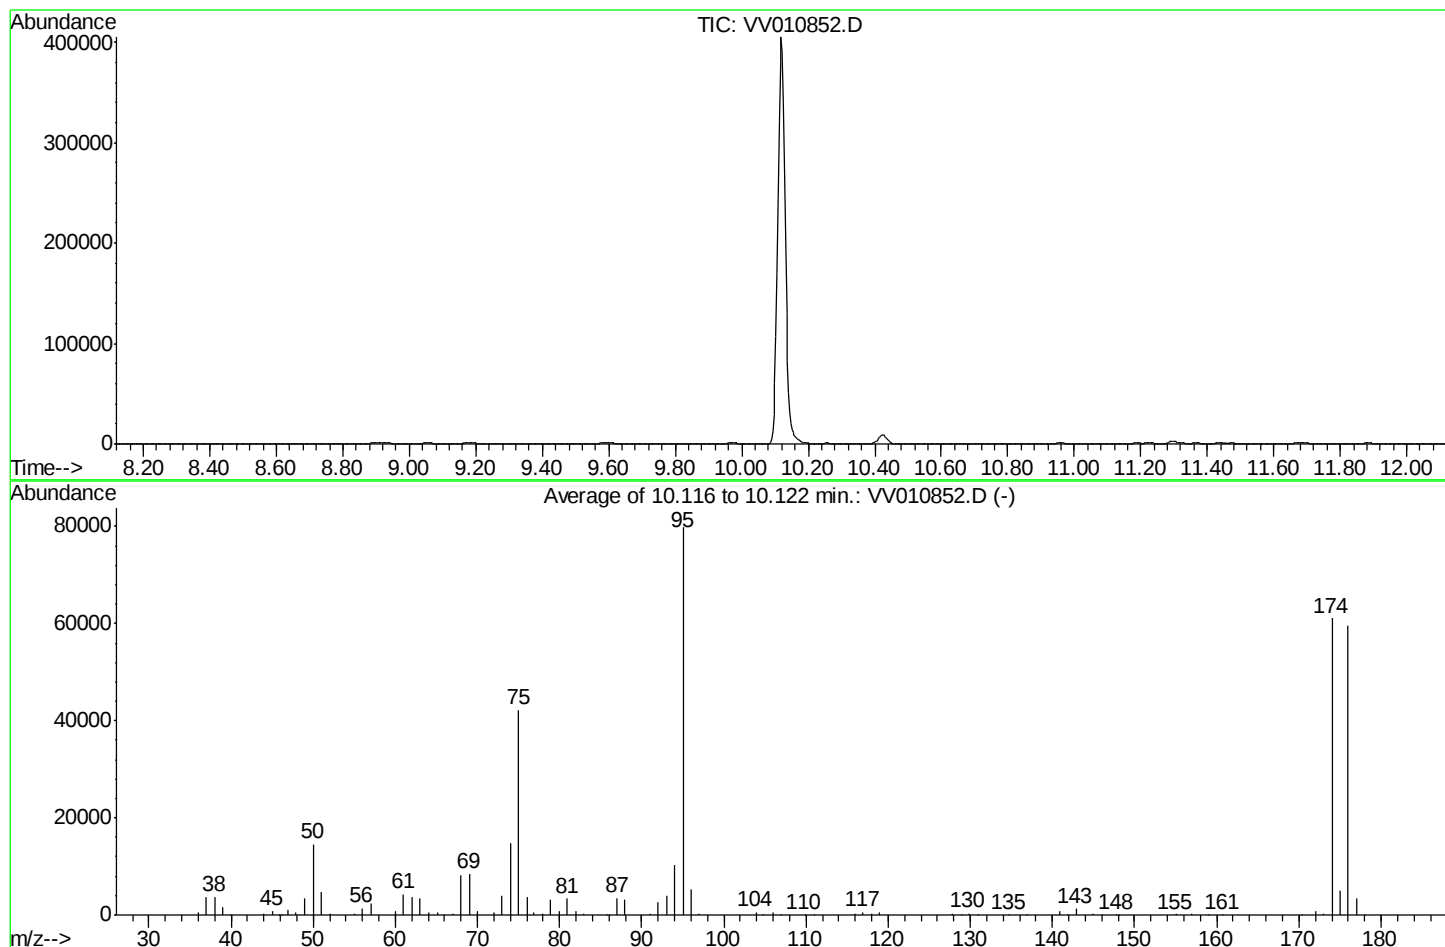

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	14584	PASS
75	95	30	80	53.0	42285	PASS
95	95	100	100	100.0	79816	PASS
96	95	5	9	6.7	5334	PASS
173	174	0.00	2	0.5	325	PASS
174	95	50	120	76.5	61096	PASS
175	174	5	9	8.4	5131	PASS
176	174	95	101	97.6	59624	PASS
177	176	5	9	5.9	3514	PASS

Scan 2796 (10.080 min): VV010852.D
BFB97

m/z	Abundance
39.90	170.0
44.00	167.0

Instrument :
MSVOA_V
ClientSampleId :
BFB97

m/z	Abundance
36.10	592.0
37.00	3722.0
38.00	3616.0
39.00	1465.0
39.90	246.0
43.90	513.0
45.00	796.0
45.90	119.0
47.00	1095.0
47.90	583.0
49.00	3310.0
50.00	14229.0
51.00	4764.0
52.00	235.0
55.00	197.0
55.90	1390.0
57.00	2334.0
60.00	918.0
61.00	4147.0
62.00	3743.0
63.00	3391.0
64.00	461.0
65.10	553.0
65.90	123.0
66.90	216.0
68.00	7740.0
69.00	8492.0
70.00	706.0
71.90	498.0
73.00	3822.0
74.00	14201.0
75.00	41672.0
76.00	3902.0
76.80	440.0
78.00	282.0
78.90	3060.0
79.90	915.0
80.90	3226.0
82.00	777.0
82.90	151.0
85.70	117.0
87.00	3503.0
88.00	3171.0
90.90	355.0
92.00	2593.0
93.00	3789.0
94.00	10017.0
95.00	77840.0
96.10	5161.0
97.00	165.0
103.90	515.0
104.70	122.0
105.90	383.0
106.90	126.0
109.80	102.0
110.90	104.0
115.90	293.0
116.90	556.0
117.90	381.0
119.00	520.0
127.90	242.0
128.90	112.0
129.80	345.0
130.90	122.0
134.70	135.0
137.00	118.0
140.90	923.0
141.80	117.0
142.90	1208.0
144.90	166.0
146.00	119.0
147.80	171.0
155.10	182.0
156.90	192.0
159.00	111.0
160.80	108.0
170.30	105.0
172.00	842.0
173.00	976.0
174.00	57504.0
175.00	4862.0
176.00	56000.0
177.00	3405.0

Instrument :
MSVOA_V
ClientSampleId :
BFB97

m/z	Abundance
36.00	596.0
37.00	3776.0
38.00	3948.0
39.00	1608.0
39.90	206.0
43.90	524.0
45.00	839.0
46.20	120.0
47.00	1175.0
47.80	493.0
49.00	3441.0
50.00	15049.0
51.00	4863.0
52.00	214.0
55.00	218.0
56.00	1454.0
57.00	2368.0
60.00	821.0
61.00	4451.0
62.00	3858.0
63.00	3509.0
64.00	462.0
65.10	547.0
66.90	197.0
68.00	8462.0
69.00	8878.0
70.00	718.0
71.90	490.0
73.00	4162.0
74.00	15381.0
75.00	43888.0
76.00	3873.0
76.80	503.0
77.90	259.0
78.90	3246.0
79.90	925.0
80.90	3463.0
82.00	795.0
83.00	168.0
86.00	139.0
87.00	3622.0
88.00	3330.0
90.90	348.0
92.00	2773.0
93.00	3971.0
94.00	10697.0
95.00	82432.0
96.00	5605.0
97.00	156.0
103.90	559.0
104.70	115.0
106.00	401.0
107.00	124.0
115.90	336.0
116.90	583.0
118.00	391.0
118.90	528.0
127.80	268.0
128.90	117.0
129.80	330.0
130.80	114.0
134.70	140.0
136.80	126.0
140.90	936.0
142.90	1335.0
144.90	200.0
146.00	117.0
147.80	169.0
155.10	196.0
157.00	199.0
159.00	100.0
160.80	149.0
170.30	127.0
172.00	831.0
174.00	62976.0
175.00	5293.0
176.00	61776.0
177.00	3606.0
177.90	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB97

m/z	Abundance
36.00	560.0
37.00	3490.0
38.00	3709.0
39.00	1568.0
39.80	184.0
44.00	566.0
45.00	806.0
46.20	135.0
47.00	1107.0
47.80	421.0
49.00	3391.0
50.00	14476.0
51.00	4462.0
52.00	189.0
55.10	236.0
56.00	1316.0
57.00	2193.0
60.00	706.0
61.00	4229.0
62.00	3747.0
63.00	3114.0
64.00	380.0
65.10	500.0
67.00	193.0
68.00	8499.0
69.00	8351.0
70.00	679.0
72.00	466.0
73.00	3979.0
74.00	14765.0
75.00	41296.0
76.00	3471.0
76.90	467.0
77.90	277.0
78.90	3057.0
80.00	896.0
80.90	3359.0
82.00	691.0
83.00	141.0
86.00	165.0
87.00	3291.0
87.90	3156.0
91.00	294.0
92.00	2623.0
93.00	3803.0
94.00	10328.0
95.00	79176.0
96.00	5237.0
97.00	154.0
103.90	515.0
104.70	100.0
105.90	433.0
115.90	370.0
117.00	589.0
117.90	351.0
118.90	504.0
127.70	312.0
128.90	124.0
129.80	343.0
130.90	110.0
134.70	126.0
136.80	135.0
140.90	866.0
142.90	1253.0
144.90	190.0
146.00	109.0
148.00	168.0
155.00	223.0
157.00	183.0
160.70	146.0
170.40	124.0
172.00	705.0
174.00	62808.0
175.00	5238.0
176.00	61096.0
177.00	3533.0
178.00	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB97