
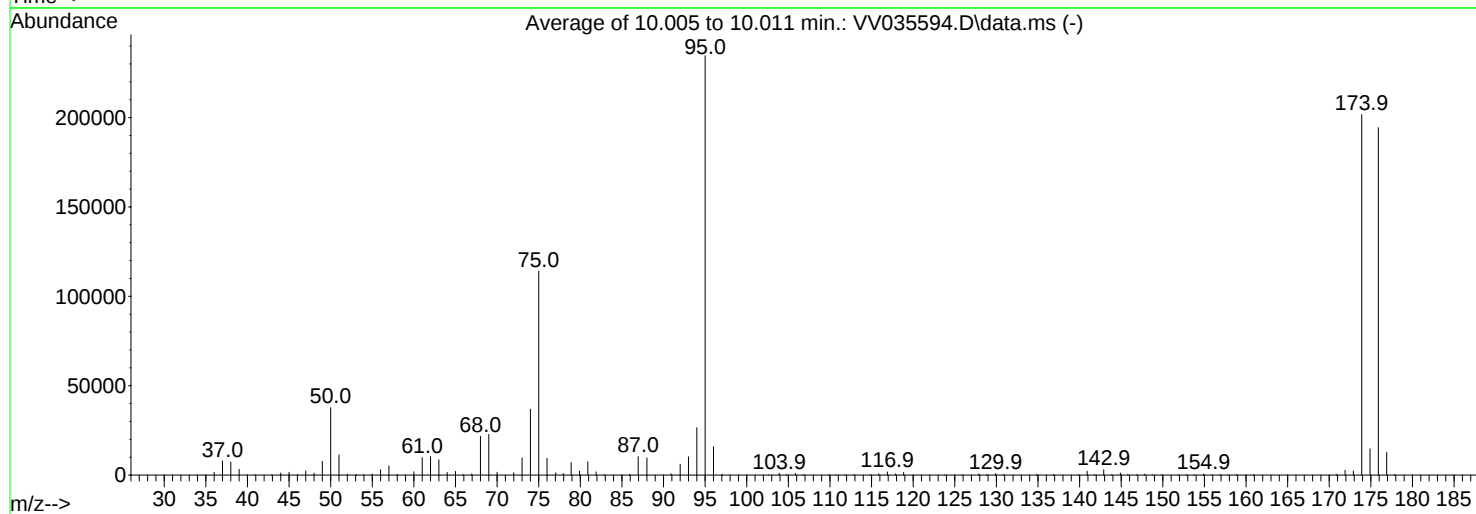


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051424\
Data File : VV035594.D
Acq On : 13 May 2024 12:01
Operator : SY/MD
Sample : BFB206
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB206

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM051024.M
Title : TRACE VOA SOM01.0
Last Update : Sat May 11 01:09:31 2024

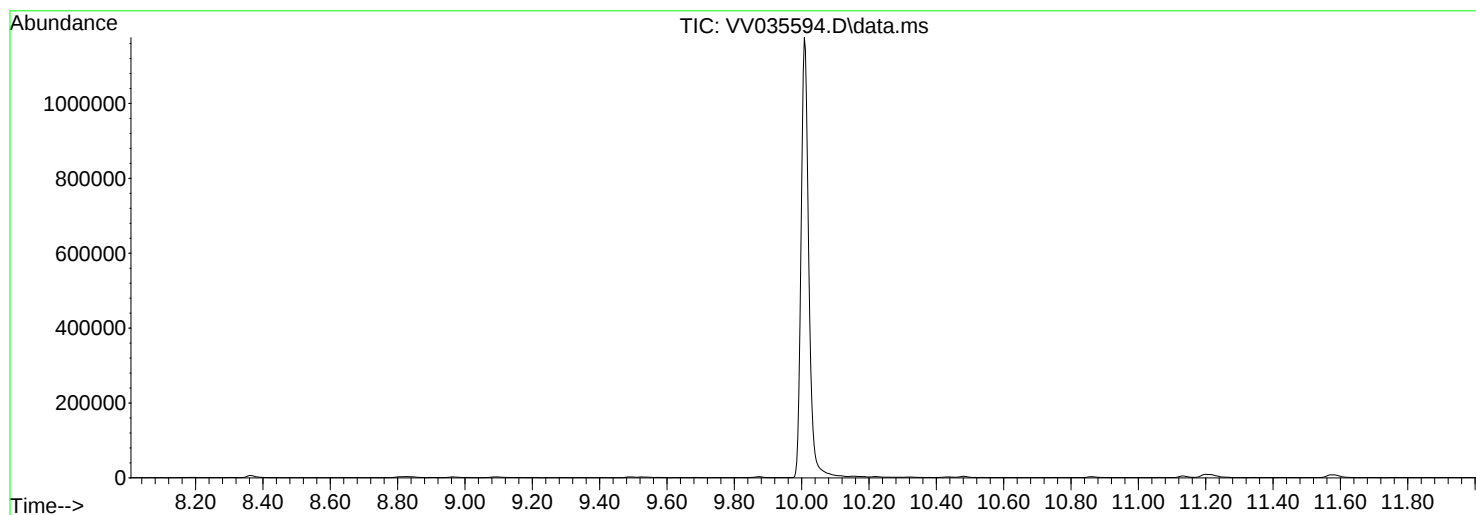

AutoFind: Scans 2788, 2789, 2790; Background Corrected with Scan 2776

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	37688	PASS
75	95	30	80	48.6	114035	PASS
95	95	100	100	100.0	234603	PASS
96	95	5	9	6.8	15843	PASS
173	174	0.00	2	1.1	2284	PASS
174	95	50	120	86.0	201685	PASS
175	174	5	9	7.3	14695	PASS
176	174	95	101	96.4	194368	PASS
177	176	5	9	6.5	12693	PASS

m/z	Abundance
39.90	311.0
44.00	546.0

Instrument :
MSVOA_V
ClientSampleId :
BFB206

m/z	Abundance
36.00	1577.0
37.00	7552.0
38.00	7059.0
39.00	3338.0
40.00	344.0
40.90	126.0
44.00	1702.0
45.00	1673.0
46.10	357.0
47.00	2227.0
48.00	977.0
49.00	7575.0
50.00	36928.0
51.00	11006.0
52.00	509.0
53.10	226.0
53.90	127.0
55.00	578.0
56.00	2902.0
57.00	5132.0
58.10	258.0
60.00	1801.0
61.00	9639.0
62.00	9958.0
63.00	8375.0
64.00	1464.0
65.00	2095.0
65.90	270.0
66.90	595.0
68.00	20984.0
69.00	22376.0
70.00	1498.0
72.00	1212.0
73.00	9434.0
74.00	35920.0
75.00	110304.0
76.00	9063.0
77.00	1214.0
77.90	895.0
78.90	6989.0
79.90	2088.0
80.90	7317.0
81.90	1810.0
82.80	213.0
85.90	411.0
87.00	9931.0
88.00	9099.0
90.90	721.0
92.00	5846.0
93.00	9724.0
94.00	25696.0
95.00	225408.0
96.00	15214.0
97.00	411.0
102.60	114.0
103.90	937.0
104.80	333.0
105.90	866.0
106.80	324.0
109.80	123.0
110.70	113.0
111.70	169.0
112.90	189.0
114.80	223.0
115.80	723.0
116.90	1734.0
117.90	700.0
118.90	1484.0
123.80	142.0
127.90	679.0
128.90	328.0
129.90	830.0
130.90	346.0
134.80	320.0
136.80	387.0
139.90	190.0
140.90	2002.0
141.80	251.0
142.90	2792.0
143.90	202.0
144.90	1369.0
145.80	426.0
146.80	115.0
147.80	445.0
148.70	143.0
149.80	205.0
151.80	130.0
152.80	213.0
153.80	167.0
154.90	625.0
155.90	124.0
156.90	395.0

Instrument :
MSVOA_V
ClientSampleId :
BFB206

157.80	123.0
159.00	248.0
160.90	218.0
170.90	503.0
171.90	2655.0
172.90	2179.0
173.90	188032.0
174.90	13912.0
175.90	180352.0
176.90	11919.0
177.90	314.0

Instrument :
MSVOA_V
ClientSampleId :
BFB206

m/z	Abundance
36.00	1689.0
37.00	8146.0
38.00	7613.0
39.00	3310.0
40.00	338.0
40.90	105.0
44.00	1751.0
45.00	1668.0
46.00	370.0
47.00	2371.0
48.00	1123.0
49.00	7940.0
50.00	38968.0
51.00	11713.0
52.00	616.0
53.10	299.0
53.90	127.0
55.00	593.0
56.00	3063.0
57.00	5375.0
57.90	235.0
60.00	1901.0
61.00	10178.0
62.00	10715.0
63.00	8948.0
64.00	1488.0
65.00	2157.0
65.90	264.0
67.00	652.0
68.00	22512.0
69.00	23680.0
70.00	1670.0
72.00	1367.0
73.00	9966.0
74.00	38192.0
75.00	118592.0
76.00	9748.0
77.10	1334.0
78.00	871.0
78.90	7254.0
79.90	2317.0
80.90	7718.0
81.90	1842.0
82.80	210.0
85.90	472.0
86.90	10752.0
88.00	9917.0
90.90	814.0
92.00	6285.0
93.00	10616.0
94.00	27496.0
95.00	243136.0
96.00	16544.0
97.10	405.0
102.70	103.0
103.90	1045.0
104.80	363.0
105.80	967.0
106.80	307.0
109.80	118.0
110.70	111.0
111.80	163.0
112.90	179.0
114.80	226.0
115.80	744.0
116.90	1854.0
117.90	778.0
118.90	1500.0
123.80	138.0
127.90	750.0
128.80	382.0
129.90	943.0
130.90	395.0
134.80	370.0
136.80	408.0
139.80	213.0
140.90	2278.0
141.80	269.0
142.90	3123.0
143.80	183.0
144.90	1261.0
145.80	458.0
146.80	144.0
147.80	505.0
148.80	192.0
149.80	238.0
151.80	179.0
152.80	189.0
153.80	176.0
154.90	666.0
155.90	125.0
156.90	404.0

Instrument :
MSVOA_V
ClientSampleId :
BFB206

157.70	115.0
158.80	244.0
160.90	260.0
170.90	534.0
171.90	2781.0
172.90	2367.0
173.90	209024.0
174.90	15282.0
175.90	201728.0
176.90	13145.0
177.90	316.0

Instrument : MSVOA_V
ClientSampleId : BFB206

m/z	Abundance
36.00	1569.0
37.00	7832.0
38.00	7406.0
39.00	3057.0
40.00	308.0
42.90	126.0
44.00	1715.0
45.00	1451.0
46.00	330.0
47.00	2229.0
48.00	1052.0
49.00	7558.0
50.00	37168.0
51.00	11193.0
52.00	654.0
53.10	312.0
54.00	130.0
55.00	538.0
56.00	2977.0
57.00	5074.0
57.90	215.0
60.00	1886.0
61.00	9536.0
62.00	10384.0
63.00	8350.0
64.00	1391.0
65.00	1978.0
65.90	235.0
67.00	603.0
68.00	21416.0
69.00	22376.0
70.00	1640.0
72.00	1310.0
73.00	9403.0
74.00	36488.0
75.00	113208.0
76.00	9487.0
77.00	1348.0
77.90	845.0
78.90	6916.0
79.90	2272.0
80.90	7187.0
81.90	1739.0
82.90	188.0
85.90	416.0
86.90	10262.0
88.00	9640.0
90.90	859.0
92.00	6168.0
93.00	10254.0
94.00	26336.0
95.00	235264.0
96.00	15772.0
97.10	374.0
102.70	101.0
103.90	1017.0
104.80	333.0
105.90	958.0
106.80	258.0
110.70	127.0
111.90	191.0
112.90	165.0
114.80	182.0
115.90	717.0
116.90	1726.0
117.90	741.0
118.80	1414.0
123.80	120.0
125.80	107.0
127.90	767.0
128.80	399.0
129.90	864.0
130.90	369.0
134.90	392.0
136.90	378.0
139.80	175.0
140.90	2212.0
141.80	233.0
142.90	2982.0
143.80	172.0
144.90	982.0
145.80	404.0
146.90	187.0
147.80	518.0
148.80	223.0
149.80	249.0
151.80	184.0
152.80	161.0
153.70	168.0
154.90	567.0
155.90	102.0
156.90	395.0

Instrument :
MSVOA_V
ClientSampleId :
BFB206

157.70	111.0
158.80	235.0
160.90	255.0
170.80	484.0
171.90	2616.0
172.90	2306.0
173.90	208000.0
174.90	14892.0
175.90	201024.0
176.90	13015.0
177.80	334.0

Instrument :
MSVOA_V
ClientSampleId :
BFB206