

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051524\
 Data File : VV035607.D
 Acq On : 14 May 2024 13:20
 Operator : SY/MD
 Sample : P2416-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHAS3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051424WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV035607.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	66	73	90	rVB	102620	116717	16.09%	1.863%
2	1.532	145	153	164	rVB	97738	111623	15.39%	1.781%
3	2.056	306	316	337	rVB	173758	251926	34.72%	4.020%
4	2.446	427	437	450	rBV	20064	35525	4.90%	0.567%
5	2.963	587	598	614	rVB3	5929	12190	1.68%	0.195%
6	3.828	851	867	906	rBV2	51390	281397	38.79%	4.491%
7	4.246	981	997	1031	rVB2	124613	339113	46.74%	5.412%
8	4.953	1200	1217	1247	rBV2	282303	725517	100.00%	11.578%
9	5.532	1385	1397	1427	rBV	246779	526462	72.56%	8.401%
10	5.828	1474	1489	1515	rBV2	15445	37015	5.10%	0.591%
11	5.986	1526	1538	1567	rBV	165137	353988	48.79%	5.649%
12	6.915	1818	1827	1856	rBV	63516	132775	18.30%	2.119%
13	7.243	1916	1929	1952	rBV	287943	531502	73.26%	8.482%
14	7.558	2018	2027	2054	rBV2	36227	77171	10.64%	1.231%
15	7.873	2112	2125	2136	rBV2	6559	12792	1.76%	0.204%
16	8.027	2164	2173	2219	rBV	285878	665313	91.70%	10.617%
17	8.783	2397	2408	2442	rBV	398403	683273	94.18%	10.904%
18	10.153	2822	2834	2856	rBV	112442	183973	25.36%	2.936%
19	10.323	2877	2887	2899	rVB	15858	24638	3.40%	0.393%
20	10.857	3045	3053	3064	rBV2	4718	7527	1.04%	0.120%
21	11.181	3144	3154	3179	rBV	374261	598021	82.43%	9.543%
22	11.558	3261	3271	3297	rVB	308472	508426	70.08%	8.113%
23	12.294	3491	3500	3518	rBV5	9786	18490	2.55%	0.295%
24	12.616	3594	3600	3610	rVB5	9018	14498	2.00%	0.231%
25	13.204	3774	3783	3795	rBV5	5105	8242	1.14%	0.132%
26	13.448	3850	3859	3868	rBV2	4882	8347	1.15%	0.133%




Sum of corrected areas: 6266461

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051524\
Data File : VV035607.D
Acq On : 14 May 2024 13:20
Operator : SY/MD
Sample : P2416-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHAS3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051424WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

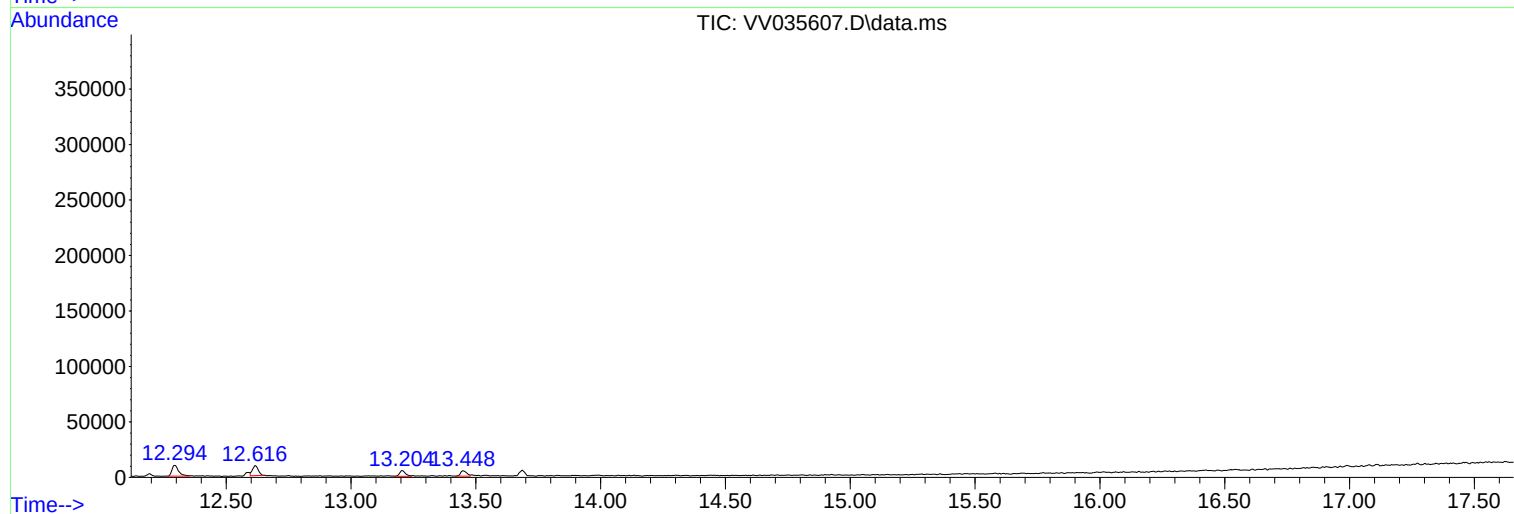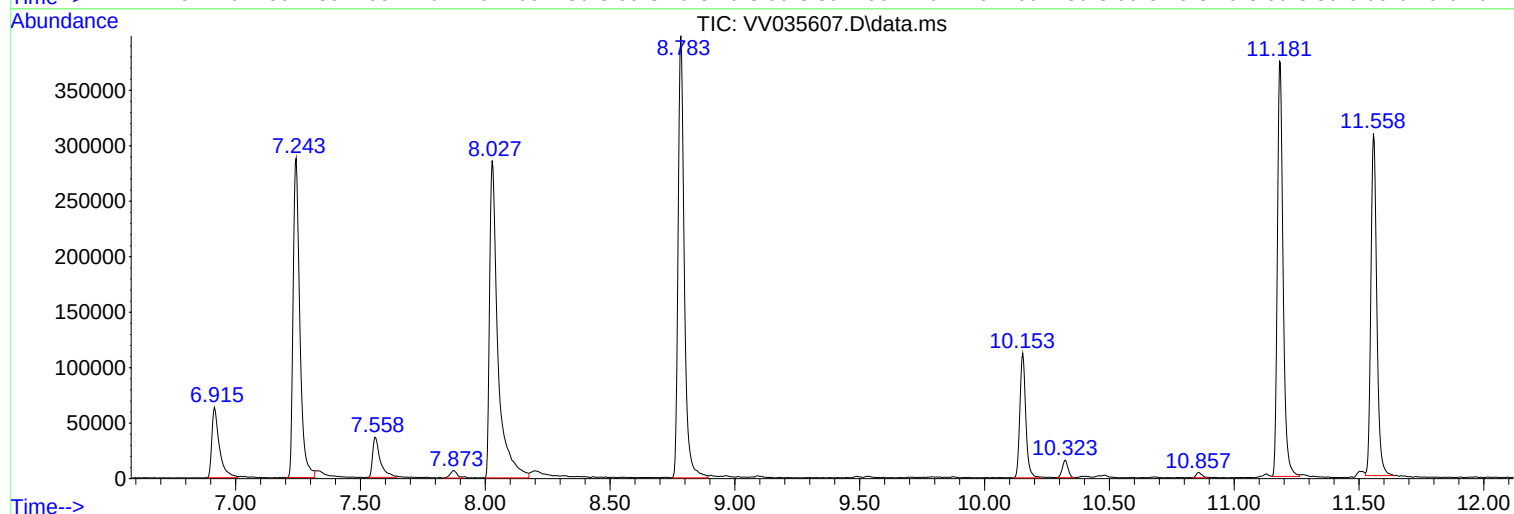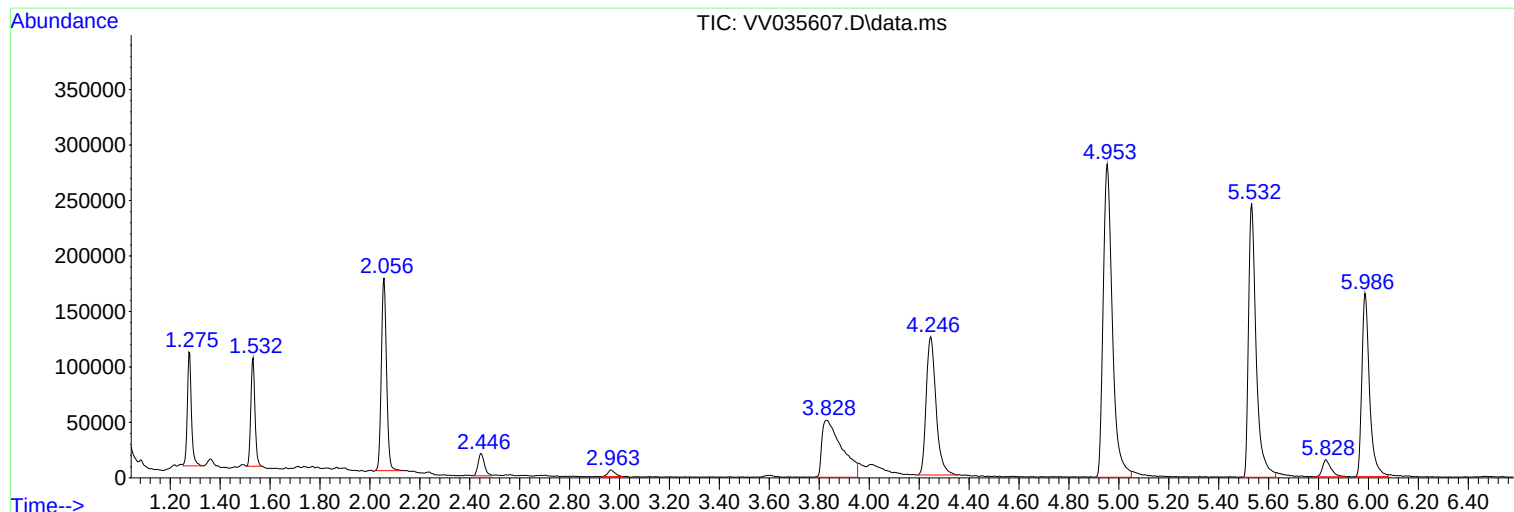

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051524\
Data File : VV035607.D
Acq On : 14 May 2024 13:20
Operator : SY/MD
Sample : P2416-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHAS3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051424WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051524\
Data File : VV035607.D
Acq On : 14 May 2024 13:20
Operator : SY/MD
Sample : P2416-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHAS3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051424WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
