

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051524\
 Data File : VV035608.D
 Acq On : 14 May 2024 13:43
 Operator : SY/MD
 Sample : P2416-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHAS4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051424WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV035608.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	91	rVB	99938	113092	15.64%	1.768%
2	1.356	93	98	113	rVB	8970	14029	1.94%	0.219%
3	1.532	145	153	168	rVB	95515	114388	15.82%	1.789%
4	2.057	306	316	332	rBV	165493	242744	33.57%	3.796%
5	2.449	429	438	452	rVB2	6537	12067	1.67%	0.189%
6	3.815	850	863	908	rBV3	72228	314319	43.47%	4.915%
7	4.024	919	928	951	rVB4	5883	18943	2.62%	0.296%
8	4.249	983	998	1033	rVB	126647	338460	46.81%	5.293%
9	4.957	1203	1218	1257	rBV2	276256	723028	100.00%	11.306%
10	5.535	1387	1398	1425	rBV	238385	520061	71.93%	8.132%
11	5.831	1479	1490	1512	rBV3	13754	33492	4.63%	0.524%
12	5.989	1526	1539	1570	rBV	163237	353206	48.85%	5.523%
13	6.918	1818	1828	1853	rBV	62760	131510	18.19%	2.056%
14	7.243	1918	1929	1953	rBV	281810	519830	71.90%	8.129%
15	7.561	2018	2028	2051	rBV2	36316	75785	10.48%	1.185%
16	7.876	2114	2126	2145	rVB	18227	34497	4.77%	0.539%
17	8.027	2164	2173	2212	rBV	323246	684480	94.67%	10.703%
18	8.783	2397	2408	2435	rBV	392988	681260	94.22%	10.653%
19	10.153	2823	2834	2853	rBV	115407	189998	26.28%	2.971%
20	10.323	2876	2887	2899	rBV	57799	94210	13.03%	1.473%
21	10.857	3045	3053	3065	rBV2	4526	7603	1.05%	0.119%
22	11.185	3144	3155	3176	rBV	369342	596172	82.45%	9.323%
23	11.503	3244	3254	3261	rBV4	6118	11679	1.62%	0.183%
24	11.558	3261	3271	3306	rVB	310152	514325	71.13%	8.043%
25	12.194	3458	3469	3479	rBV2	11924	19982	2.76%	0.312%
26	12.291	3491	3499	3511	rBV7	10816	20282	2.81%	0.317%
27	12.616	3592	3600	3611	rVB4	9043	15517	2.15%	0.243%




Sum of corrected areas: 6394959

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051524\
Data File : VV035608.D
Acq On : 14 May 2024 13:43
Operator : SY/MD
Sample : P2416-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHAS4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051424WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

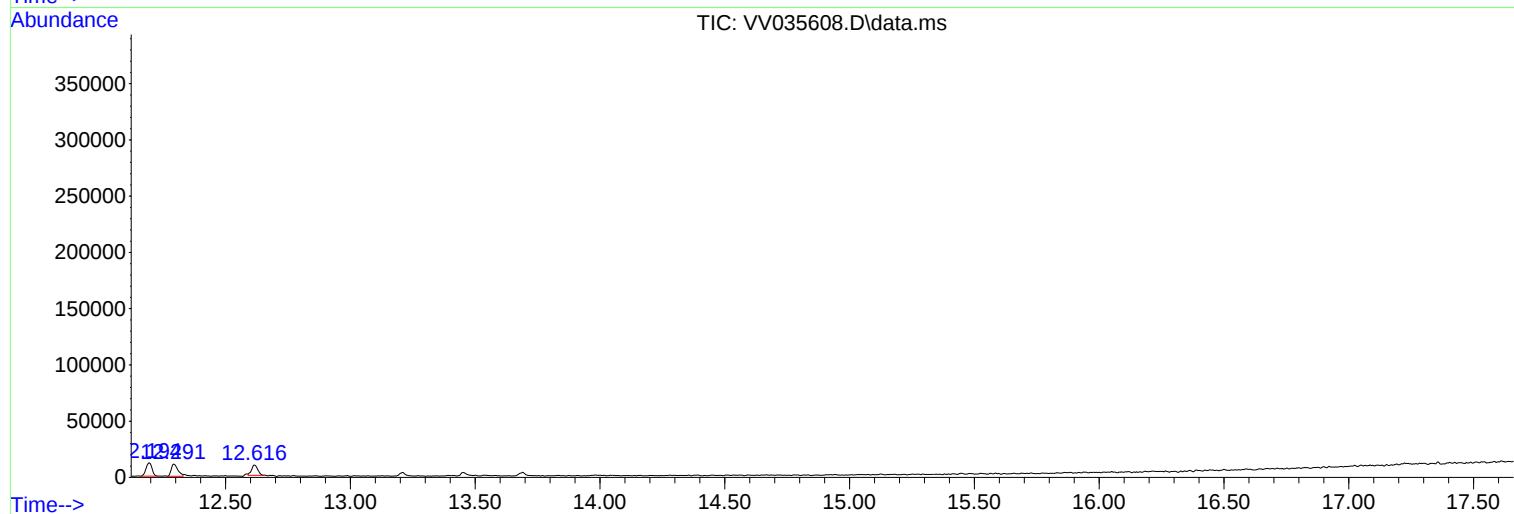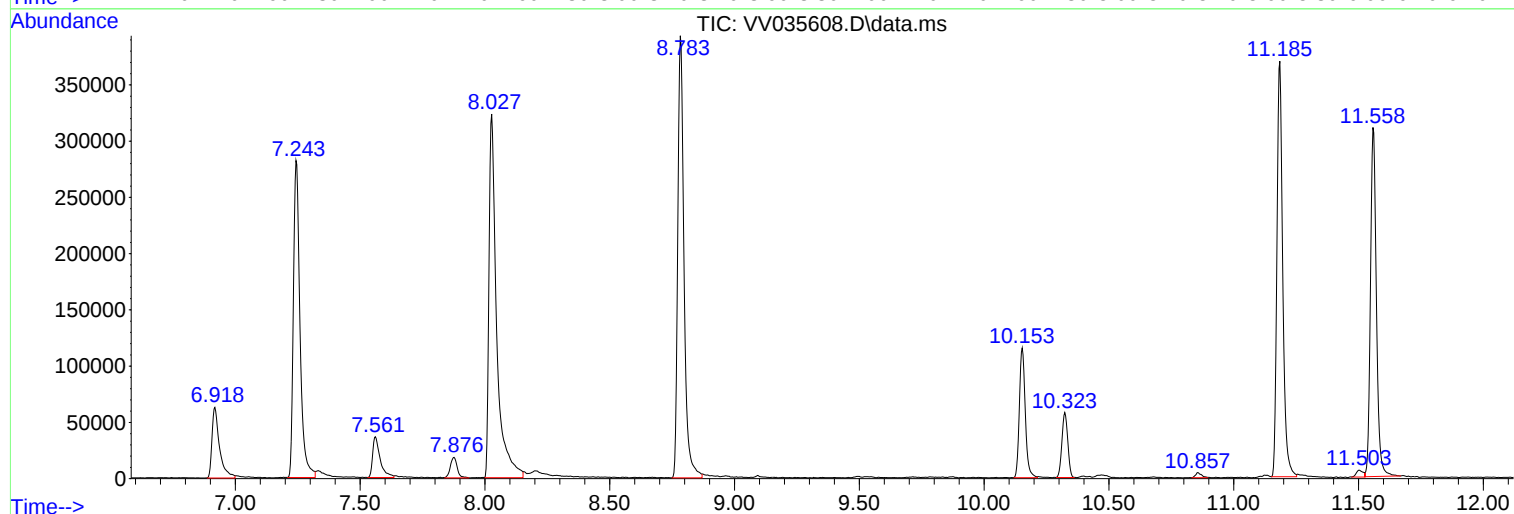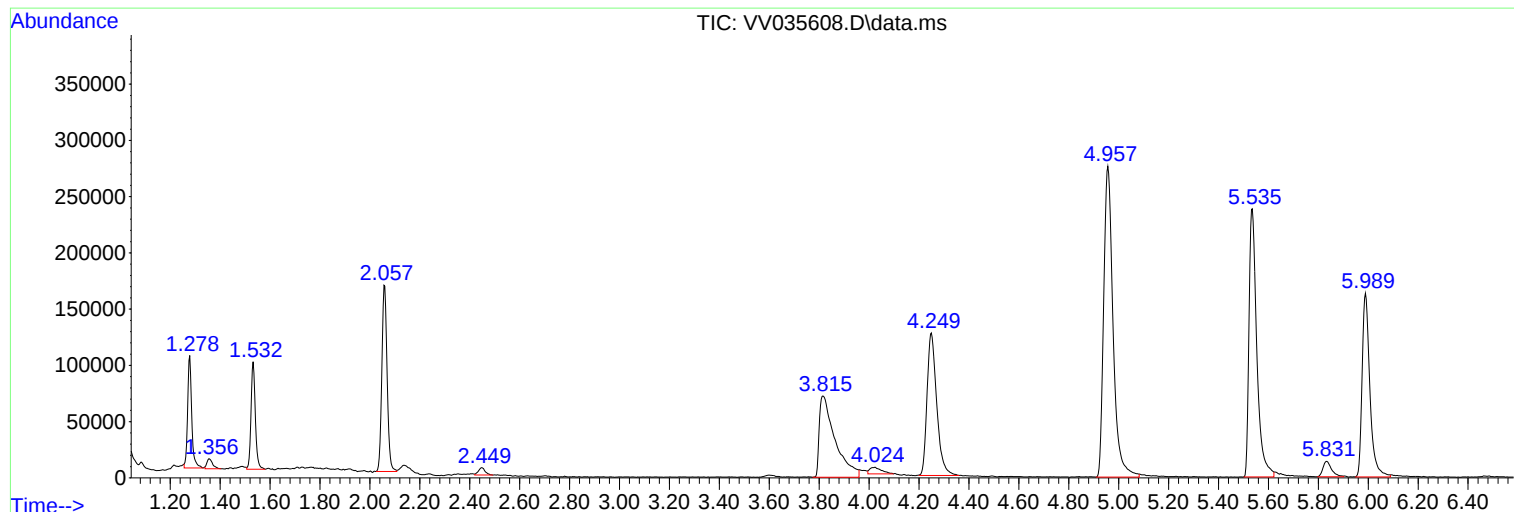

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051524\
Data File : VV035608.D
Acq On : 14 May 2024 13:43
Operator : SY/MD
Sample : P2416-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHAS4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051424WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051524\
Data File : VV035608.D
Acq On : 14 May 2024 13:43
Operator : SY/MD
Sample : P2416-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHAS4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051424WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc