
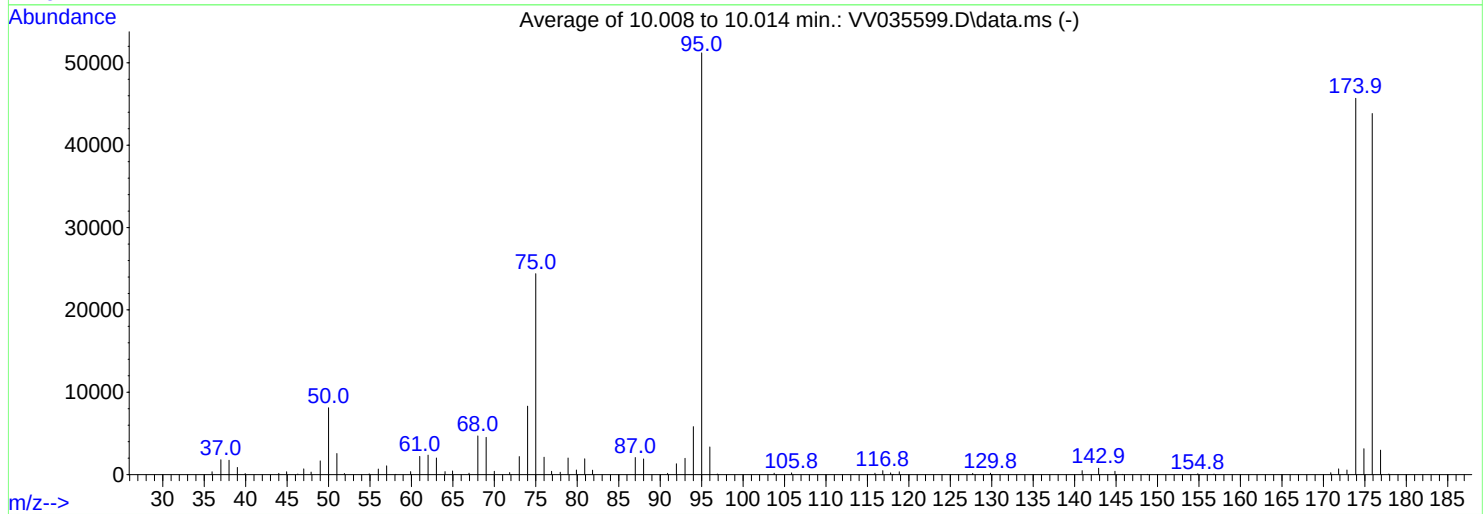


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051524\
Data File : VV035599.D
Acq On : 14 May 2024 09:18
Operator : SY/MD
Sample : BFB271
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB271

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051424WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu May 16 01:35:17 2024

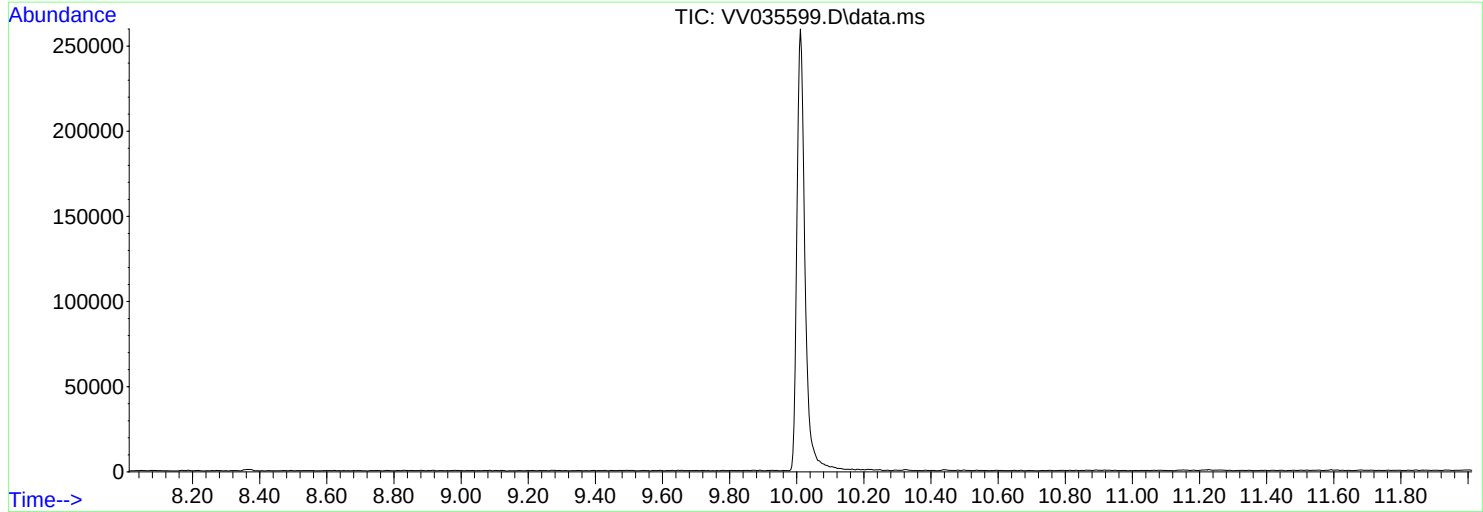

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.8	8114	PASS
75	95	30	80	47.6	24392	PASS
95	95	100	100	100.0	51211	PASS
96	95	5	9	6.5	3352	PASS
173	174	0.00	2	1.2	562	PASS
174	95	50	120	89.2	45696	PASS
175	174	5	9	6.9	3153	PASS
176	174	95	105	96.0	43853	PASS
177	176	5	10	6.8	2966	PASS

m/z	Abundance
40.00	136.0
44.00	599.0

Instrument :
MSVOA_V
ClientSampleId :
BFB271

m/z	Abundance
36.00	356.0
37.00	1858.0
38.00	1796.0
39.00	838.0
40.00	254.0
44.00	701.0
45.00	359.0
47.00	718.0
47.90	340.0
49.00	1662.0
50.00	8383.0
51.00	2667.0
51.90	153.0
54.90	155.0
56.00	697.0
57.00	1089.0
59.90	365.0
61.00	2302.0
62.00	2445.0
63.00	2083.0
64.00	396.0
65.00	453.0
67.00	184.0
68.00	4589.0
69.00	4366.0
70.00	429.0
71.80	241.0
73.00	2197.0
74.00	8049.0
75.00	24200.0
76.00	2156.0
76.90	445.0
77.90	319.0
78.90	1923.0
79.90	568.0
80.90	1826.0
81.80	536.0
87.00	2148.0
88.00	1818.0
90.80	149.0
91.90	1295.0
93.00	2009.0
94.00	5873.0
95.00	51048.0
96.00	3409.0
96.90	114.0
103.80	180.0
105.90	200.0
115.90	184.0
116.90	469.0
117.90	256.0
118.80	298.0
127.70	129.0
129.90	186.0
140.90	482.0
142.90	786.0
144.80	424.0
145.80	102.0
148.80	103.0
154.90	109.0
170.90	255.0
171.80	684.0
172.90	549.0
173.90	44448.0
174.90	3144.0
175.90	42352.0
176.90	2902.0
177.90	125.0

Instrument :
MSVOA_V
ClientSampleId :
BFB271

m/z	Abundance
36.00	358.0
37.00	1852.0
38.00	1832.0
39.00	919.0
39.90	261.0
44.00	779.0
44.90	377.0
46.30	106.0
47.00	732.0
47.90	342.0
49.00	1759.0
50.00	8316.0
51.00	2648.0
51.90	146.0
54.90	137.0
56.00	708.0
57.00	1109.0
58.10	117.0
59.90	357.0
61.00	2277.0
62.00	2427.0
63.00	2006.0
64.10	393.0
65.00	440.0
66.90	185.0
68.00	4887.0
69.00	4675.0
70.00	423.0
71.90	268.0
73.00	2315.0
74.00	8634.0
75.00	25288.0
76.00	2169.0
76.90	425.0
78.00	299.0
78.90	2083.0
79.90	568.0
80.90	1950.0
81.90	529.0
87.00	2129.0
88.00	1975.0
90.90	156.0
91.90	1371.0
93.00	2042.0
94.00	6029.0
95.00	53112.0
96.00	3449.0
96.90	100.0
103.70	170.0
105.90	205.0
115.90	185.0
116.90	522.0
117.80	216.0
118.80	349.0
127.70	157.0
129.80	186.0
140.90	514.0
142.90	810.0
144.80	413.0
154.90	120.0
156.80	119.0
170.90	264.0
171.90	707.0
172.90	586.0
173.90	47216.0
174.90	3240.0
175.90	45360.0
176.90	3079.0
177.90	122.0

Instrument :
MSVOA_V
ClientSampleId :
BFB271

m/z	Abundance
35.90	353.0
37.00	1683.0
38.00	1637.0
39.00	845.0
39.90	281.0
44.00	780.0
44.90	308.0
46.30	130.0
47.00	670.0
47.90	282.0
49.00	1597.0
50.00	7643.0
51.00	2410.0
51.90	127.0
56.00	663.0
57.00	1035.0
59.90	368.0
61.00	2070.0
62.00	2258.0
63.00	1959.0
64.00	335.0
64.90	442.0
66.90	153.0
68.00	4652.0
69.00	4545.0
70.00	370.0
71.90	258.0
73.00	2082.0
74.00	8251.0
75.00	23688.0
76.00	2057.0
76.90	355.0
78.00	239.0
78.90	2046.0
79.90	545.0
80.90	1995.0
81.90	550.0
87.00	1957.0
88.00	1912.0
91.00	163.0
92.00	1285.0
93.00	1923.0
94.00	5595.0
95.00	49472.0
96.00	3198.0
103.70	174.0
105.80	214.0
115.90	170.0
116.80	491.0
117.70	157.0
118.10	133.0
118.90	409.0
127.70	170.0
129.80	173.0
140.90	460.0
142.90	754.0
144.90	395.0
154.80	113.0
156.80	114.0
170.90	189.0
171.90	719.0
172.80	550.0
173.90	45424.0
174.90	3074.0
175.90	43848.0
176.90	2917.0

Instrument :
MSVOA_V
ClientSampleId :
BFB271