
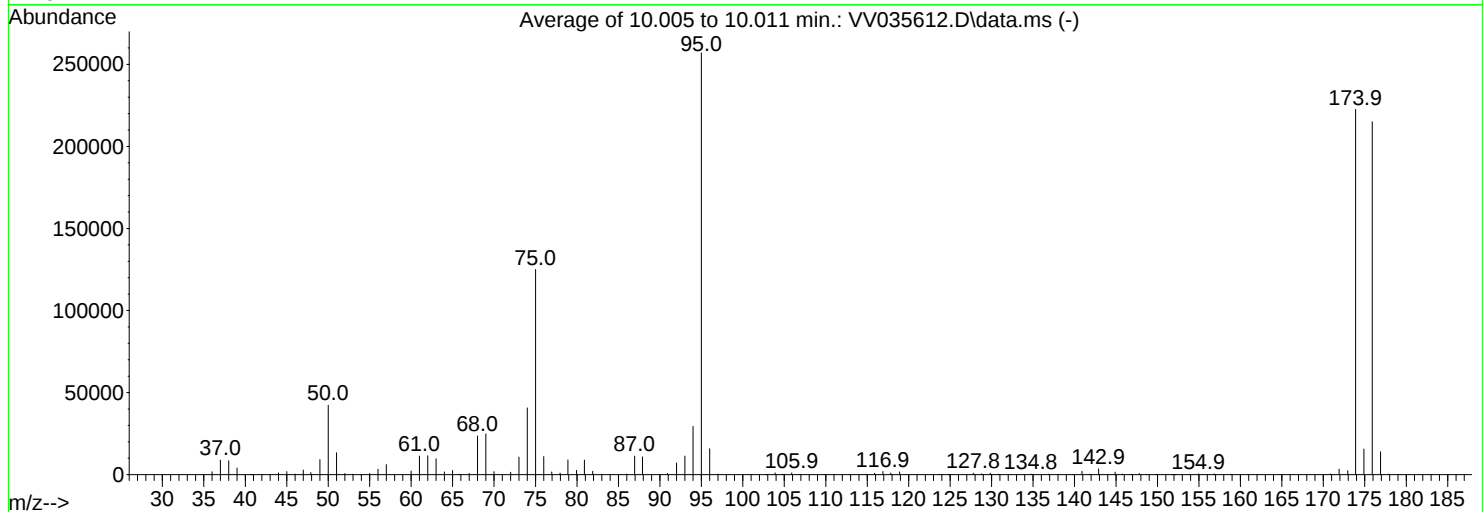


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051524\
Data File : VV035612.D
Acq On : 15 May 2024 08:28
Operator : SY/MD
Sample : BFB272
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB272

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051424WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu May 16 01:35:17 2024

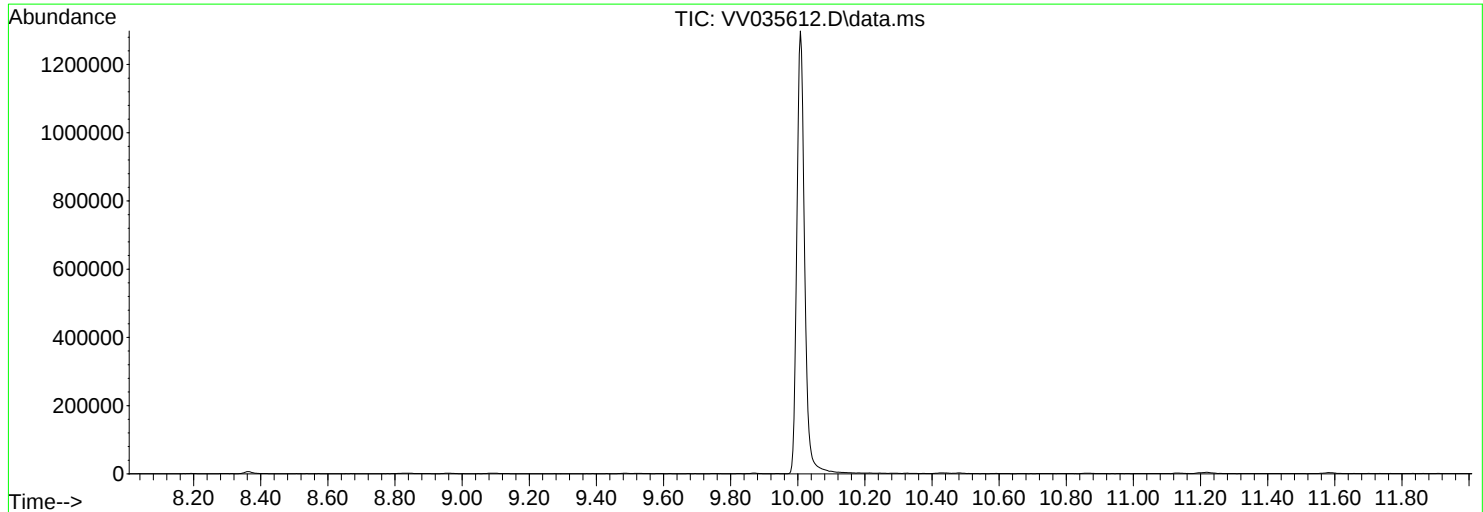

AutoFind: Scans 2788, 2789, 2790; Background Corrected with Scan 2776

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	42280	PASS
75	95	30	80	48.6	124976	PASS
95	95	100	100	100.0	257024	PASS
96	95	5	9	6.1	15786	PASS
173	174	0.00	2	1.0	2327	PASS
174	95	50	120	86.6	222549	PASS
175	174	5	9	7.0	15600	PASS
176	174	95	105	96.7	215125	PASS
177	176	5	10	6.5	13937	PASS

m/z	Abundance
39.80	214.0
44.00	449.0

Instrument :
MSVOA_V
ClientSampleId :
BFB272

m/z	Abundance
36.00	1748.0
37.00	8905.0
38.00	8818.0
39.00	3914.0
39.90	424.0
40.60	220.0
42.10	128.0
42.90	130.0
44.00	1422.0
45.00	1833.0
46.00	357.0
47.00	2934.0
47.90	1300.0
49.00	9461.0
50.00	42552.0
51.00	13194.0
52.00	693.0
52.90	299.0
53.90	179.0
55.00	691.0
56.00	3449.0
57.00	5900.0
57.90	301.0
60.00	2393.0
61.00	11437.0
62.00	11638.0
63.00	9674.0
64.00	1733.0
65.00	2583.0
65.90	277.0
67.00	632.0
68.00	23616.0
69.00	24432.0
70.00	1851.0
72.00	1547.0
73.00	10552.0
74.00	40680.0
75.00	124128.0
76.00	11067.0
76.90	1654.0
78.00	1029.0
78.90	9138.0
80.00	2758.0
80.90	9044.0
81.90	2115.0
82.90	259.0
86.00	424.0
86.90	11454.0
87.90	10869.0
90.90	727.0
92.00	7012.0
93.00	11015.0
94.00	28984.0
95.00	252608.0
96.00	16200.0
97.00	432.0
103.90	1078.0
104.80	358.0
105.90	1081.0
106.90	319.0
108.00	158.0
109.90	133.0
111.00	219.0
112.00	139.0
112.90	180.0
114.80	300.0
115.90	895.0
116.90	1899.0
117.80	913.0
118.90	1618.0
123.70	185.0
127.80	890.0
128.80	453.0
129.90	827.0
130.80	343.0
134.80	434.0
136.90	385.0
139.90	109.0
140.90	2093.0
141.90	310.0
142.90	3544.0
143.90	240.0
144.90	1730.0
145.80	472.0
146.90	147.0
147.80	581.0
148.70	112.0
149.90	278.0
152.90	159.0
153.90	213.0
155.00	537.0
156.90	448.0

Instrument :
MSVOA_V
ClientSampleId :
BFB272

158.90	273.0
160.90	241.0
170.80	572.0
171.90	3260.0
172.90	2341.0
173.90	212608.0
174.90	15021.0
175.90	204992.0
176.90	13651.0
177.90	380.0

Instrument :
MSVOA_V
ClientSampleId :
BFB272

m/z	Abundance
36.00	1786.0
37.00	9061.0
38.00	8814.0
39.00	4088.0
39.90	332.0
40.60	204.0
42.10	132.0
42.90	124.0
44.00	1555.0
45.00	1997.0
46.00	418.0
47.00	2959.0
47.90	1348.0
49.00	9462.0
50.00	43504.0
51.00	13847.0
52.00	697.0
52.90	330.0
54.10	196.0
55.00	692.0
56.00	3455.0
57.00	6369.0
57.90	279.0
60.00	2315.0
61.00	11672.0
62.00	11923.0
63.00	9996.0
64.00	1684.0
65.00	2587.0
65.90	281.0
67.00	659.0
68.00	24304.0
69.00	25888.0
70.00	1914.0
72.00	1523.0
73.00	11057.0
74.00	41968.0
75.00	129368.0
76.00	11415.0
77.00	1685.0
77.90	1050.0
78.90	9253.0
80.00	2663.0
80.90	9140.0
81.90	2142.0
82.90	276.0
86.00	460.0
86.90	11905.0
87.90	11253.0
90.90	785.0
92.00	7442.0
93.00	11648.0
94.00	30504.0
95.00	265664.0
96.00	16184.0
97.00	424.0
103.90	1104.0
104.80	365.0
105.90	1124.0
106.90	309.0
108.00	147.0
111.00	238.0
111.90	138.0
112.80	171.0
114.80	280.0
115.90	971.0
116.90	1950.0
117.90	1000.0
118.90	1706.0
123.70	172.0
124.80	101.0
127.80	912.0
128.80	512.0
129.80	887.0
130.80	303.0
134.70	450.0
136.90	470.0
139.80	148.0
140.90	2165.0
141.90	335.0
142.90	3693.0
143.90	238.0
144.90	1636.0
145.80	433.0
146.80	169.0
147.80	665.0
148.70	132.0
149.80	279.0
152.10	104.0
153.00	199.0
153.90	220.0
154.90	526.0

Instrument :
MSVOA_V
ClientSampleId :
BFB272

156.10	108.0
156.90	508.0
158.80	277.0
161.00	258.0
170.90	544.0
171.90	3491.0
172.90	2342.0
173.90	230016.0
174.90	16135.0
175.90	222720.0
176.90	14398.0
177.90	387.0

Instrument :
MSVOA_V
ClientSampleId :
BFB272

m/z	Abundance
36.00	1641.0
37.00	8562.0
38.00	7997.0
39.00	3932.0
39.90	245.0
40.80	157.0
44.00	1534.0
45.00	1849.0
46.00	445.0
47.00	2639.0
47.90	1298.0
49.00	8539.0
50.00	40784.0
51.00	13121.0
52.00	594.0
53.00	361.0
54.10	212.0
55.00	586.0
56.00	3095.0
57.00	6173.0
58.00	264.0
60.00	2173.0
61.00	10825.0
62.00	11027.0
63.00	9311.0
64.00	1536.0
65.00	2335.0
65.90	257.0
67.00	640.0
68.00	22968.0
69.00	24320.0
70.00	1766.0
72.00	1423.0
73.00	10569.0
74.00	39280.0
75.00	121432.0
76.00	10450.0
77.00	1512.0
77.90	987.0
78.90	8463.0
79.90	2386.0
80.90	8420.0
81.90	2004.0
83.00	250.0
86.00	451.0
87.00	10739.0
87.90	10461.0
90.90	793.0
92.00	7072.0
93.00	11184.0
94.00	28776.0
95.00	252800.0
96.00	14975.0
97.00	383.0
102.80	111.0
103.90	1006.0
104.80	315.0
105.90	1030.0
106.90	267.0
108.00	141.0
109.90	101.0
111.00	221.0
111.80	167.0
112.80	159.0
114.90	275.0
115.90	936.0
116.90	1935.0
117.90	1006.0
118.90	1608.0
123.90	149.0
127.80	858.0
128.80	484.0
129.80	837.0
130.90	279.0
134.70	394.0
136.90	476.0
139.70	168.0
140.90	2043.0
141.80	289.0
142.90	3423.0
143.90	195.0
144.90	1339.0
145.80	333.0
146.80	189.0
147.80	698.0
148.70	153.0
149.80	283.0
151.80	132.0
152.90	187.0
153.80	218.0
154.90	538.0
156.00	122.0

Instrument :
MSVOA_V
ClientSampleId :
BFB272

156.80	501.0
158.80	274.0
161.00	238.0
170.90	470.0
171.90	3357.0
173.00	2299.0
173.90	225024.0
174.90	15645.0
175.90	217664.0
176.90	13762.0
177.90	358.0

Instrument :
MSVOA_V
ClientSampleId :
BFB272