




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051622\
 Data File : VV025907.D
 Acq On : 16 May 2022 13:10
 Operator : SY/MD
 Sample : N2815-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 X3A80

Manual IntegrationsAPPROVED

Quant Time: May 17 08:00:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue May 17 07:58:29 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 05/17/2022
 Supervised By :Mahesh Dadoda 05/19/2022

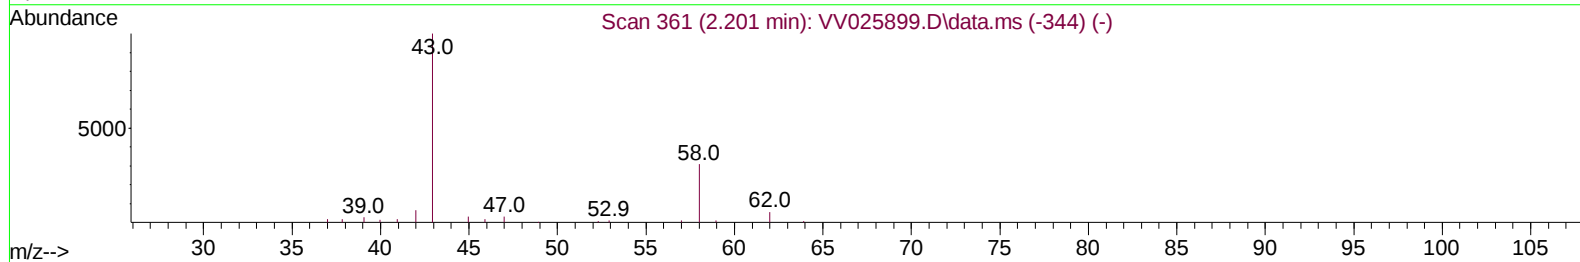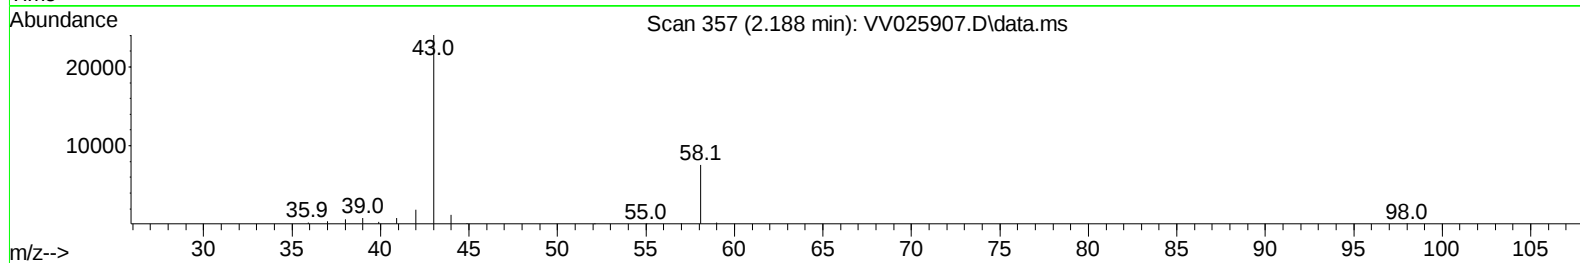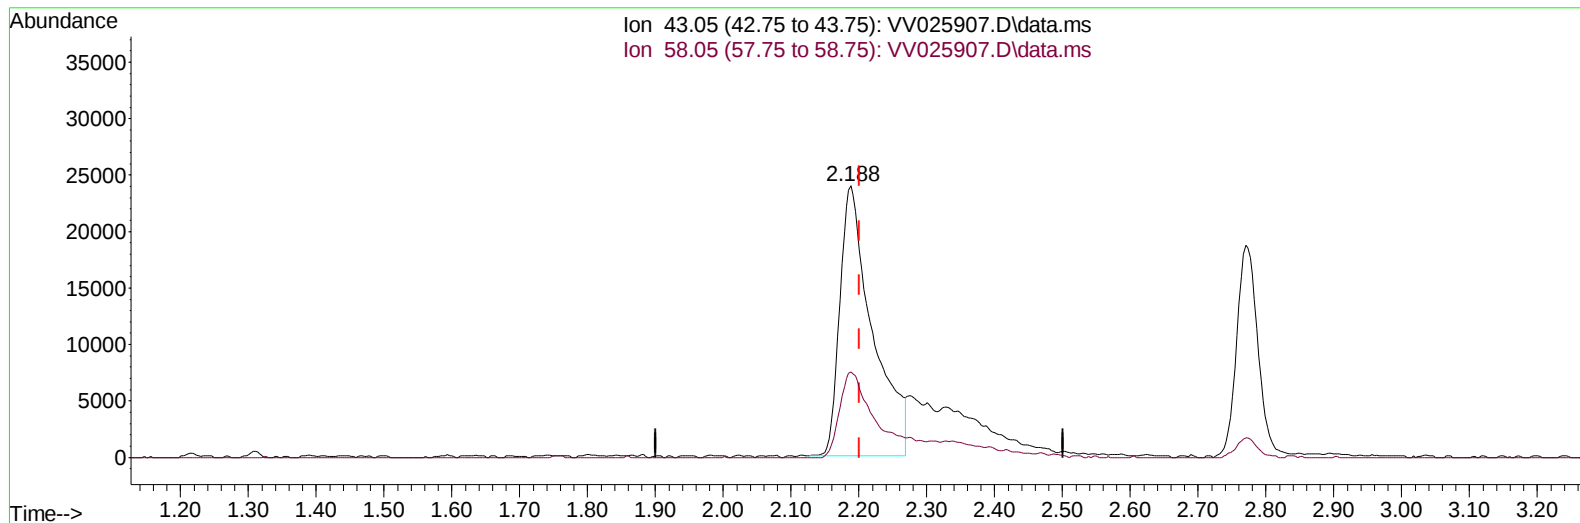

TIC: VV025907.D\data.ms

(13) Acetone (T)

2.188min (-0.013) 55.36 ug/L

response 79787

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	22.30	35.23
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051622\
 Data File : VV025907.D
 Acq On : 16 May 2022 13:10
 Operator : SY/MD
 Sample : N2815-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 X3A80

Manual IntegrationsAPPROVED

Quant Time: May 17 08:00:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue May 17 07:58:29 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 05/17/2022
 Supervised By :Mahesh Dadoda 05/19/2022

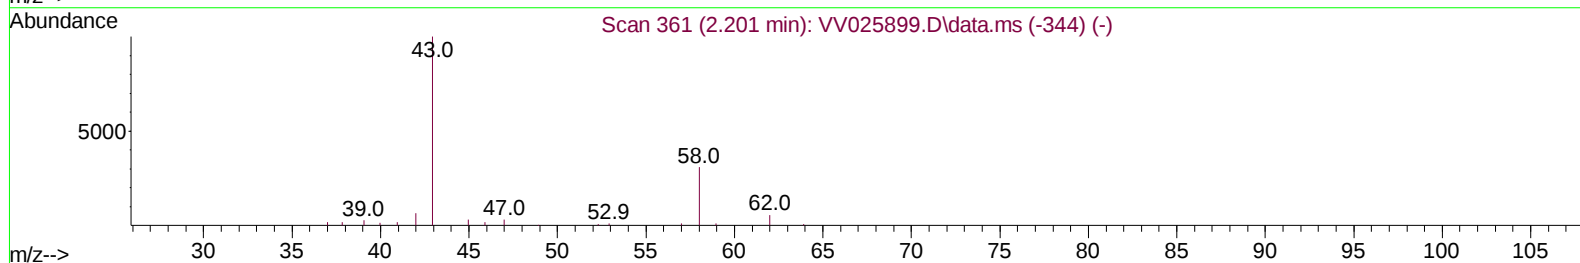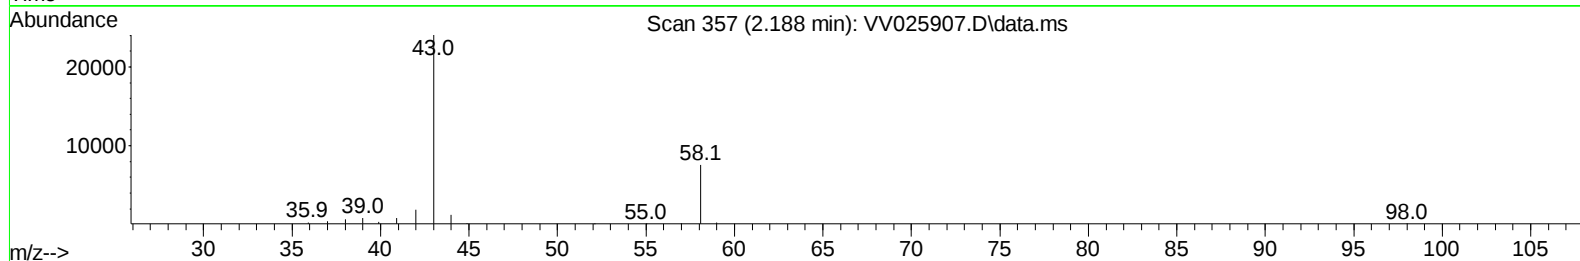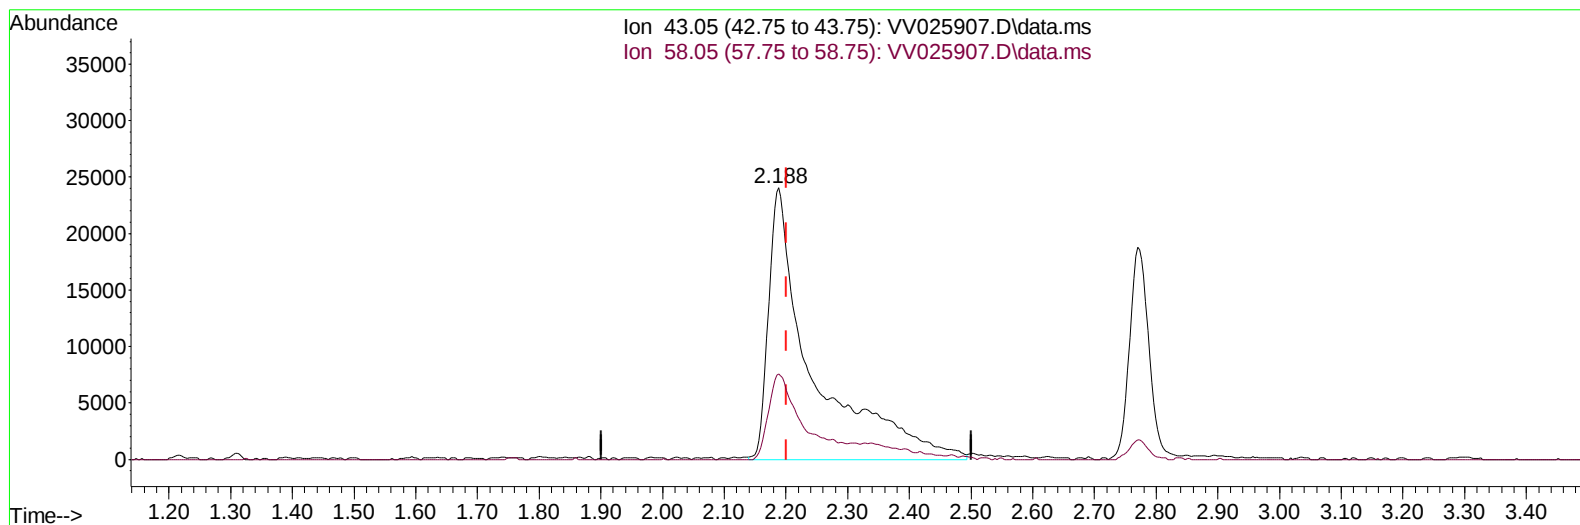

TIC: VV025907.D\data.ms

(13) Acetone (T)

2.188min (-0.013) 82.64 ug/L m

response 119104

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	22.30	23.60
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051622\
Data File : VV025907.D
Acq On : 16 May 2022 13:10
Operator : SY/MD
Sample : N2815-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
X3A80

Manual IntegrationsAPPROVED

Quant Time: May 17 08:00:48 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue May 17 07:58:29 2022
Response via : Initial Calibration

Reviewed By :John Carlone 05/17/2022
Supervised By :Mahesh Dadoda 05/19/2022

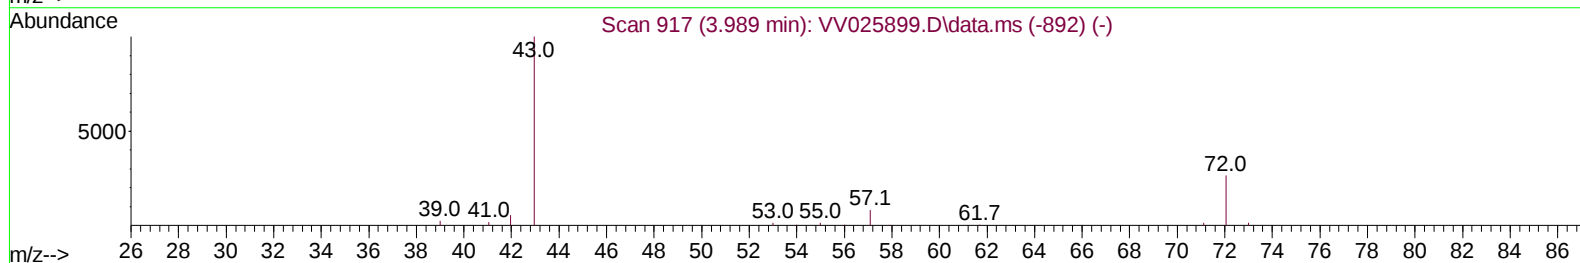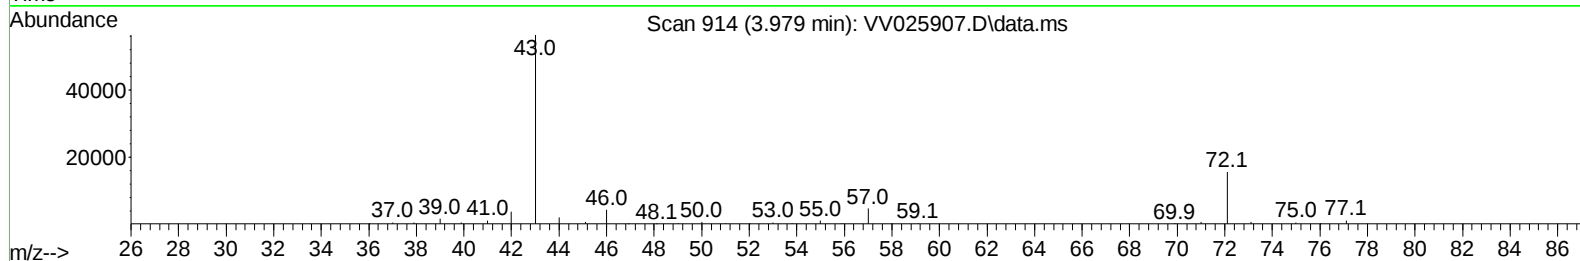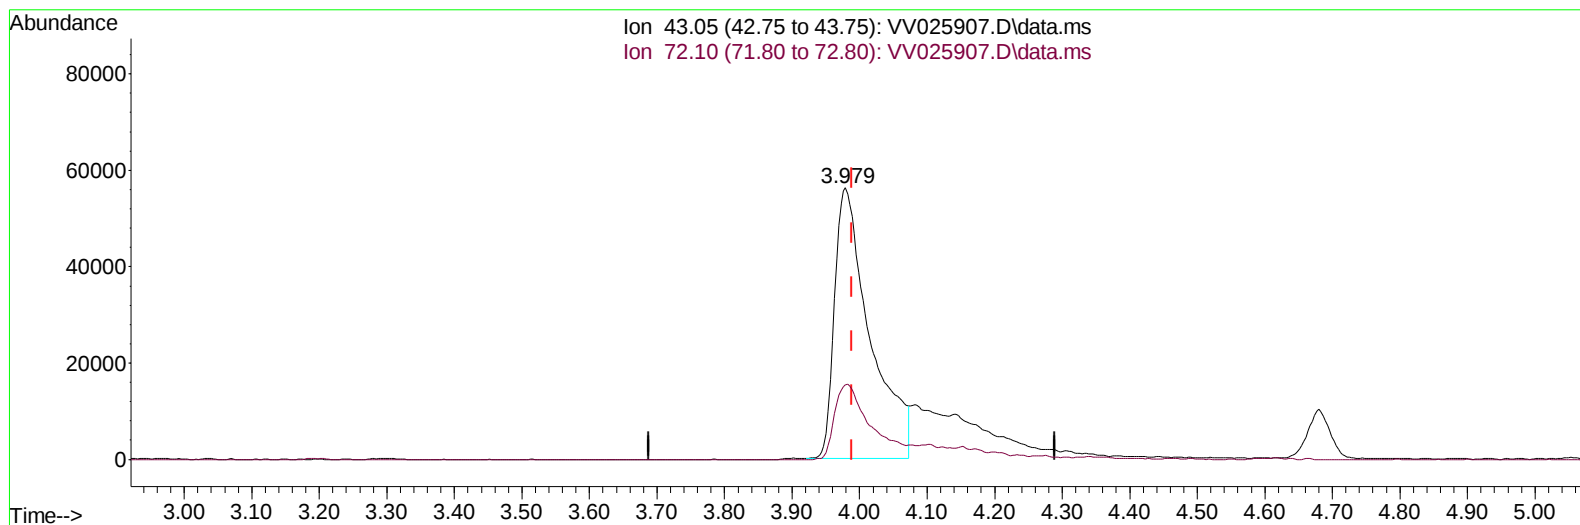

TIC: VV025907.D\data.ms

(21) 2-Butanone (T)

3.979min (-0.010) 98.76 ug/L

response 204411

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	21.10	28.16
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051622\
Data File : VV025907.D
Acq On : 16 May 2022 13:10
Operator : SY/MD
Sample : N2815-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
X3A80

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 05/17/2022
Supervised By :Mahesh Dadoda 05/19/2022

Quant Time: May 17 08:00:48 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue May 17 07:58:29 2022
Response via : Initial Calibration

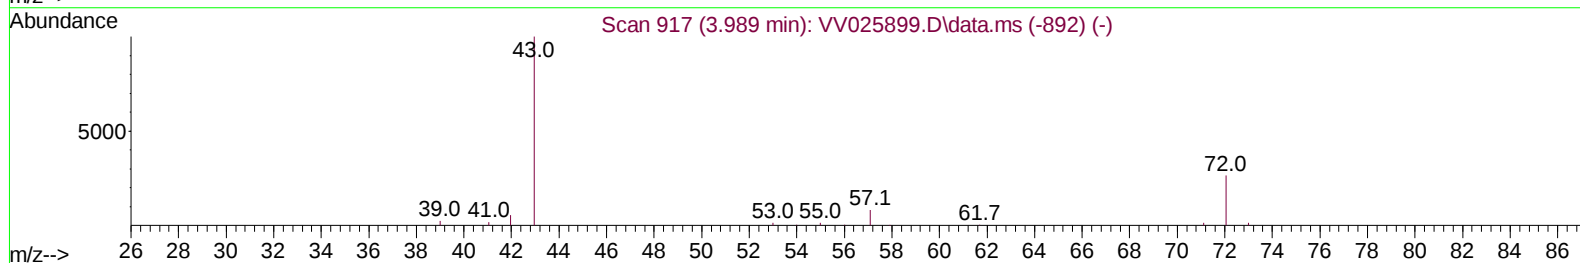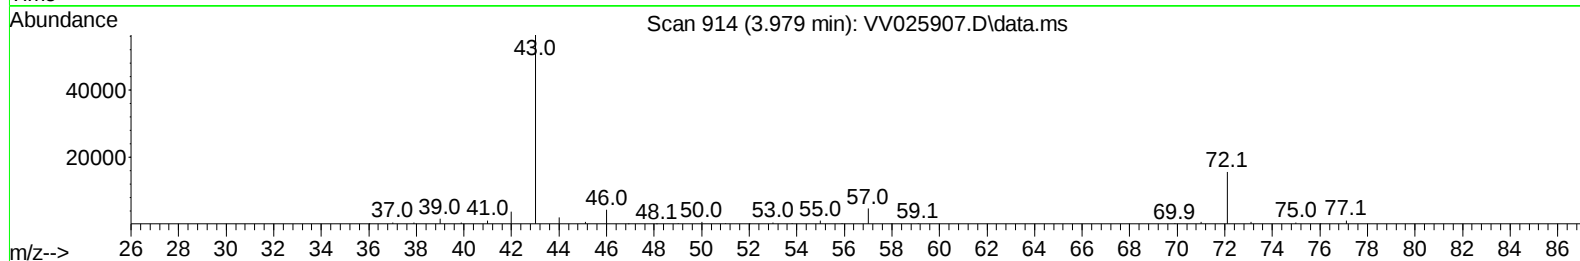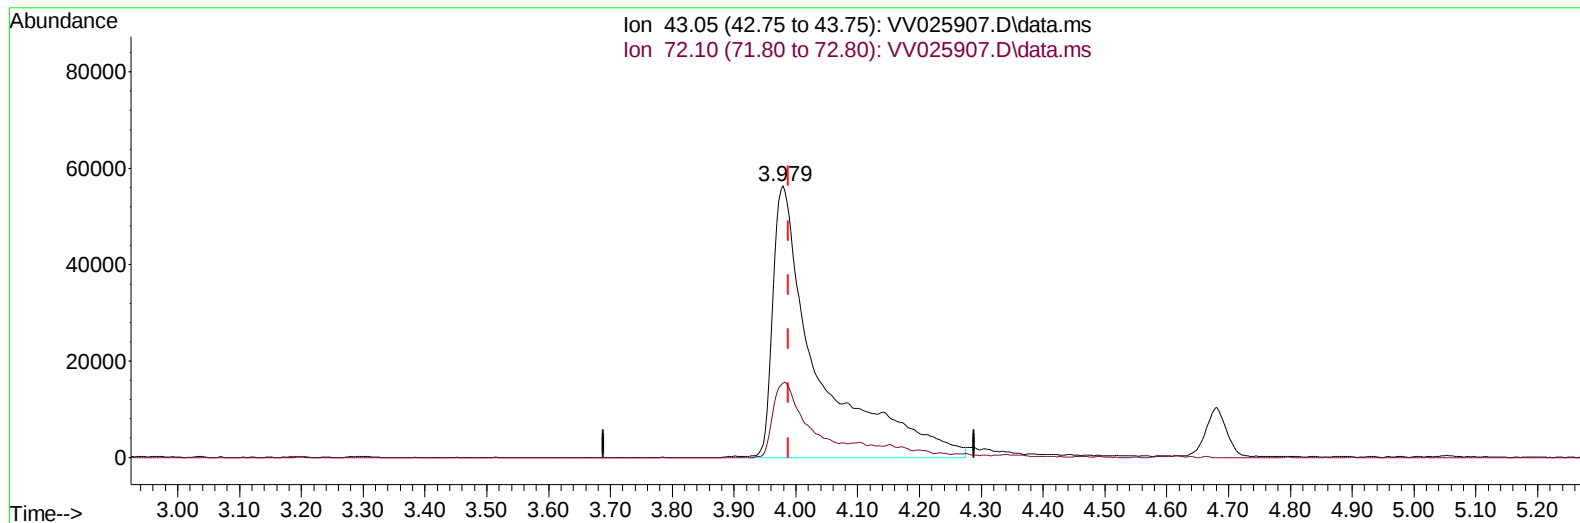

TIC: VV025907.D\data.ms

(21) 2-Butanone (T)

3.979min (-0.010) 138.89 ug/L m

response 287449

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	21.10	20.02
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051622\
 Data File : VV025907.D
 Acq On : 16 May 2022 13:10
 Operator : SY/MD
 Sample : N2815-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 X3A80

Manual IntegrationsAPPROVED

Quant Time: May 17 08:00:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue May 17 07:58:29 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 05/17/2022
 Supervised By :Mahesh Dadoda 05/19/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	156296	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	161523	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	80826	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	57322	4.441	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	88.800%	
7) Chloroethane-d5	1.571	69	54818	4.960	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	99.200%	
11) 1,1-Dichloroethene-d2	2.111	63	126117	4.414	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	88.200%	
20) 2-Butanone-d5	3.905	46	72051	48.198	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery	=	96.400%	
24) Chloroform-d	4.349	84	99228	4.706	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	94.200%	
26) 1,2-Dichloroethane-d4	5.037	65	44324	4.957	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	99.200%	
32) Benzene-d6	5.053	84	203158	4.844	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	96.800%	
36) 1,2-Dichloropropane-d6	6.072	67	58920	4.832	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	96.600%	
41) Toluene-d8	7.317	98	167168	4.287	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	85.800%	
43) trans-1,3-Dichloroprop...	7.625	79	17479	4.383	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	87.600%	
46) 2-Hexanone-d5	8.091	63	76584	51.722	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	103.440%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	40566	5.164	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	103.200%	
66) 1,2-Dichlorobenzene-d4	11.622	152	60721	5.277	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	105.600%	
Target Compounds						
						Qvalue
3) Chloromethane	1.243	50	72520	3.683	ug/L	99
6) Bromomethane	1.523	94	36907	3.061	ug/L	100
9) Trichlorofluoromethane	1.754	101	210470	7.616	ug/L	98
12) 1,1-Dichloroethene	2.121	96	57031	3.797	ug/L	85
13) Acetone	2.188	43	119104m	82.640	ug/L	
14) Carbon disulfide	2.294	76	221524	5.724	ug/L	100
16) Methylene chloride	2.510	84	35337	2.317	ug/L	98
17) Methyl tert-butyl Ether	2.770	73	219297	9.150	ug/L	99
19) 1,1-Dichloroethane	3.191	63	226369	9.128	ug/L	98
21) 2-Butanone	3.979	43	287449m	138.886	ug/L	
27) 1,2-Dichloroethane	5.133	62	102003	7.699	ug/L	100
29) 1,1,1-Trichloroethane	4.609	97	193774	8.797	ug/L	99
30) Cyclohexane	4.680	56	239152	12.193	ug/L	100
34) Trichloroethene	5.915	95	74060	5.301	ug/L	98
35) Methylcyclohexane	6.130	83	146518	6.830	ug/L	97
37) 1,2-Dichloropropane	6.178	63	27958	2.167	ug/L	99
42) Toluene	7.387	91	495630	8.704	ug/L	99
47) Tetrachloroethene	7.976	164	93730	8.658	ug/L	98

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051622\
 Data File : VV025907.D
 Acq On : 16 May 2022 13:10
 Operator : SY/MD
 Sample : N2815-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 X3A80

Manual IntegrationsAPPROVED

Reviewed By : John Carlone 05/17/2022
 Supervised By : Mahesh Dadoda 05/19/2022

Quant Time: May 17 08:00:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue May 17 07:58:29 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

48) 2-Hexanone	8.140	43	253549	60.089	ug/L	99
50) 1,2-Dibromoethane	8.352	107	132616	16.840	ug/L	98
51) Chlorobenzene	8.879	112	400949	10.855	ug/L	100
52) Ethylbenzene	9.011	91	410775	6.859	ug/L	100
53) m,p-Xylene	9.140	106	328268	14.191	ug/L	93
54) o-Xylene	9.542	106	124371	5.646	ug/L	98
55) Styrene	9.561	104	214063	5.783	ug/L	100
59) Bromoform	9.731	173	24063	5.740	ug/L	99
60) Isopropylbenzene	9.931	105	197671	3.659	ug/L	99
65) 1,4-Dichlorobenzene	11.271	146	114131	4.386	ug/L	99
67) 1,2-Dichlorobenzene	11.641	146	304783	13.271	ug/L	98
68) 1,2-Dibromo-3-chloropr...	12.429	75	5646	4.332	ug/L	93
72) 1,2,3-Trichlorobenzene	13.741	180	138960	11.137	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051622\
 Data File : VV025907.D
 Acq On : 16 May 2022 13:10
 Operator : SY/MD
 Sample : N2815-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 3

Instrument :
 MSVOA_V
 ClientSampleId :
 X3A80

Manual IntegrationsAPPROVED

Quant Time: May 17 08:00:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue May 17 07:58:29 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 05/17/2022
 Supervised By :Mahesh Dadoda 05/19/2022

