

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051622\
 Data File : VV025901.D
 Acq On : 16 May 2022 10:51
 Operator : SY/MD
 Sample : N2831-07
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YB2L6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025901.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	101	rVB	131738	135342	17.89%	2.353%
2	1.568	156	164	176	rVB	120802	136919	18.10%	2.380%
3	2.108	322	332	351	rVB	254942	366172	48.40%	6.366%
4	3.899	879	889	913	rBV2	31652	109181	14.43%	1.898%
5	4.349	1014	1029	1056	rVB2	129687	324685	42.91%	5.645%
6	5.047	1228	1246	1279	rBV2	303536	756618	100.00%	13.155%
7	5.616	1411	1423	1441	rBV	215321	434930	57.48%	7.562%
8	5.905	1502	1513	1526	rBV4	6057	13394	1.77%	0.233%
9	6.069	1551	1564	1591	rBV2	169937	355910	47.04%	6.188%
10	6.989	1838	1850	1867	rBV	70800	137594	18.19%	2.392%
11	7.313	1940	1951	1973	rBV	360822	636044	84.06%	11.058%
12	7.625	2038	2048	2062	rBV	41059	74915	9.90%	1.302%
13	7.940	2133	2146	2157	rBV2	4362	7851	1.04%	0.136%
14	8.088	2183	2192	2234	rBV	188453	490214	64.79%	8.523%
15	8.850	2418	2429	2457	rBV	340506	570495	75.40%	9.919%
16	10.214	2842	2853	2868	rBV	92411	153489	20.29%	2.669%
17	10.381	2894	2905	2916	rBV4	7064	11766	1.56%	0.205%
18	11.246	3163	3174	3197	rBV	330006	524342	69.30%	9.116%
19	11.532	3254	3263	3274	rBV3	12366	20934	2.77%	0.364%
20	11.622	3278	3291	3311	rBV	300531	475479	62.84%	8.267%
21	12.345	3506	3516	3528	rBV4	9580	15420	2.04%	0.268%




Sum of corrected areas: 5751694

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051622\
Data File : VV025901.D
Acq On : 16 May 2022 10:51
Operator : SY/MD
Sample : N2831-07
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2L6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

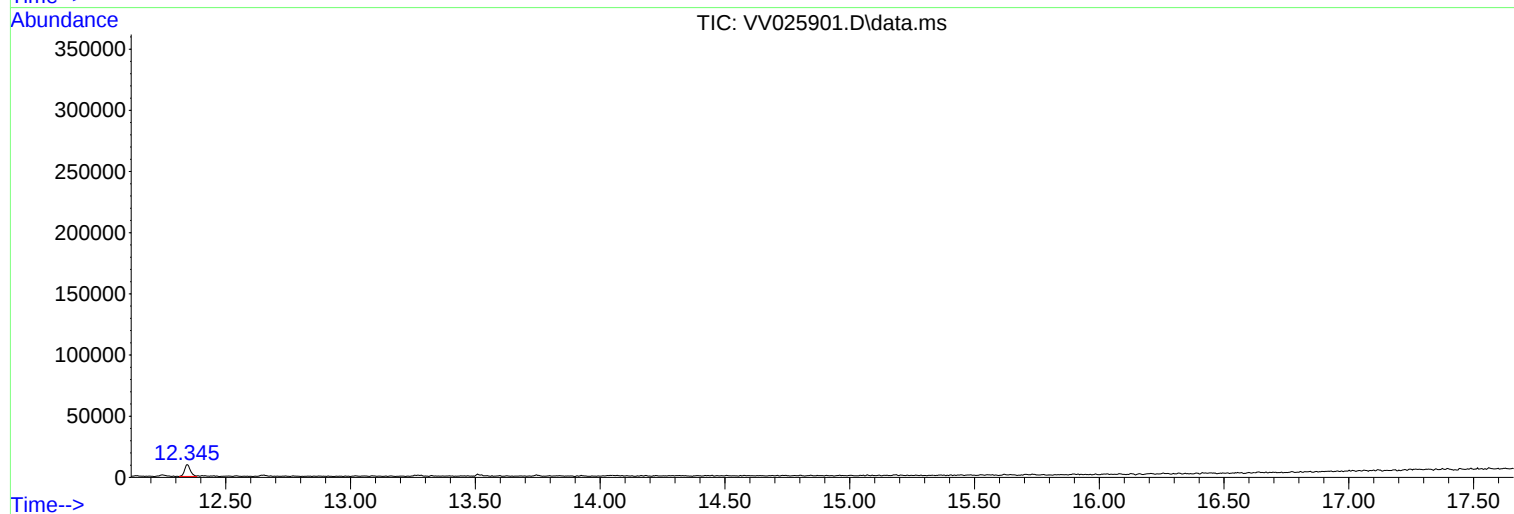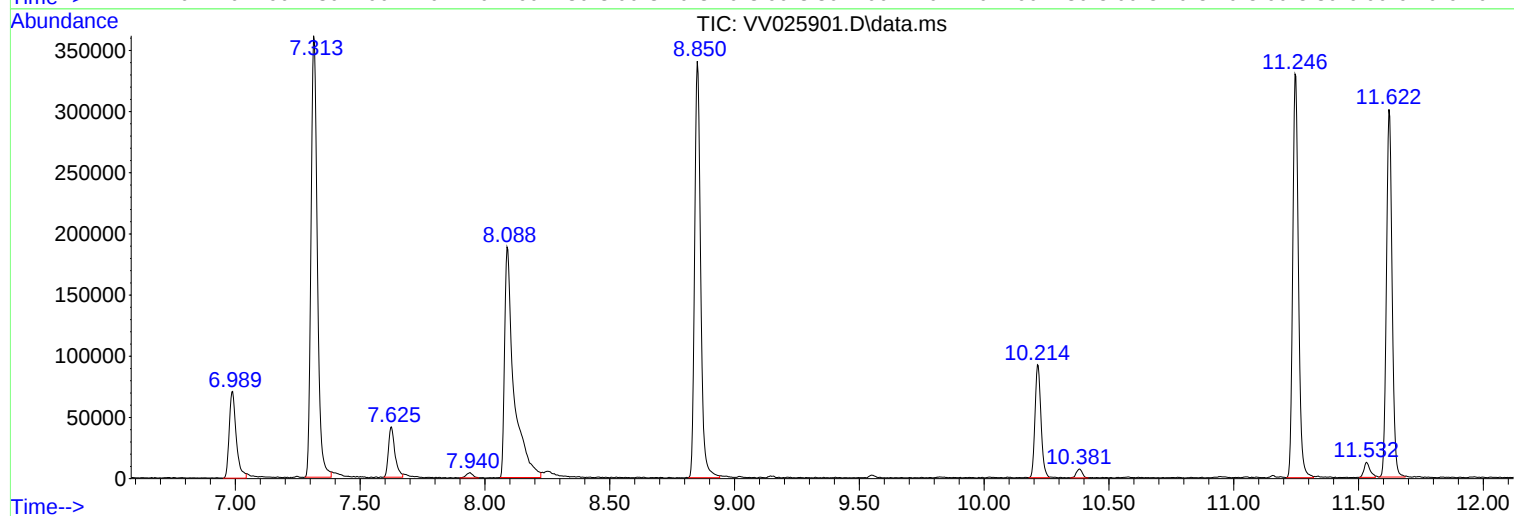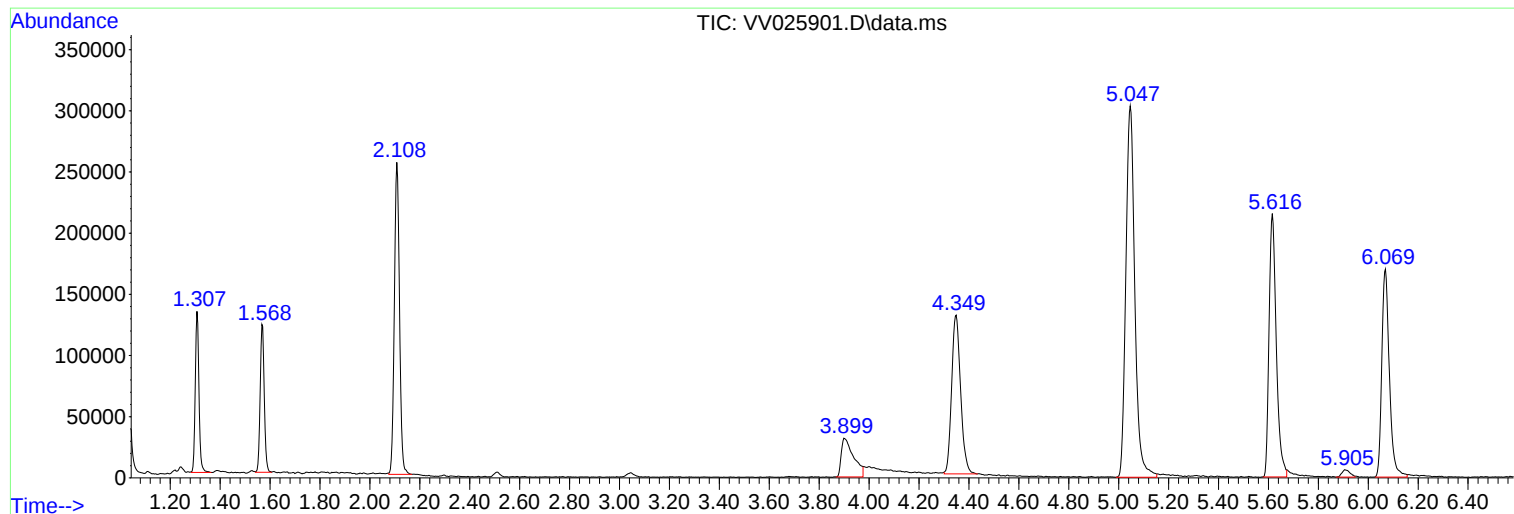

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051622\
Data File : VV025901.D
Acq On : 16 May 2022 10:51
Operator : SY/MD
Sample : N2831-07
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2L6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051622\
Data File : VV025901.D
Acq On : 16 May 2022 10:51
Operator : SY/MD
Sample : N2831-07
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2L6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc