

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051622\
 Data File : VV025902.D
 Acq On : 16 May 2022 11:15
 Operator : SY/MD
 Sample : N2831-08
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YB2L7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025902.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	74	83	96	rBV	113322	120132	19.50%	2.645%
2	1.568	156	164	176	rBV	103077	115759	18.79%	2.549%
3	2.108	318	332	353	rVB	218722	316390	51.36%	6.966%
4	3.918	884	895	916	rBV2	27124	104897	17.03%	2.309%
5	4.349	1013	1029	1059	rBV	106287	273435	44.38%	6.020%
6	5.050	1230	1247	1278	rBV2	244979	616072	100.00%	13.564%
7	5.619	1413	1424	1451	rBV	145031	300483	48.77%	6.616%
8	5.915	1504	1516	1531	rVB	4567	11006	1.79%	0.242%
9	6.072	1551	1565	1585	rBV	138153	288504	46.83%	6.352%
10	6.989	1840	1850	1866	rBV	57897	111663	18.12%	2.458%
11	7.317	1939	1952	1974	rBV	286385	513466	83.35%	11.305%
12	7.625	2039	2048	2067	rBV	32863	63274	10.27%	1.393%
13	7.944	2135	2147	2156	rBV3	4227	7127	1.16%	0.157%
14	8.091	2182	2193	2227	rBV	180958	413226	67.07%	9.098%
15	8.854	2419	2430	2455	rBV	232113	387457	62.89%	8.530%
16	10.217	2842	2854	2870	rBV	80163	130756	21.22%	2.879%
17	10.381	2895	2905	2917	rVB3	8123	13336	2.16%	0.294%
18	11.249	3165	3175	3190	rBV	229476	351246	57.01%	7.733%
19	11.532	3254	3263	3276	rBV5	4720	8376	1.36%	0.184%
20	11.622	3280	3291	3309	rBV	240477	381902	61.99%	8.408%
21	12.345	3507	3516	3528	rBV6	8678	13517	2.19%	0.298%




Sum of corrected areas: 4542024

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051622\
Data File : VV025902.D
Acq On : 16 May 2022 11:15
Operator : SY/MD
Sample : N2831-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2L7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

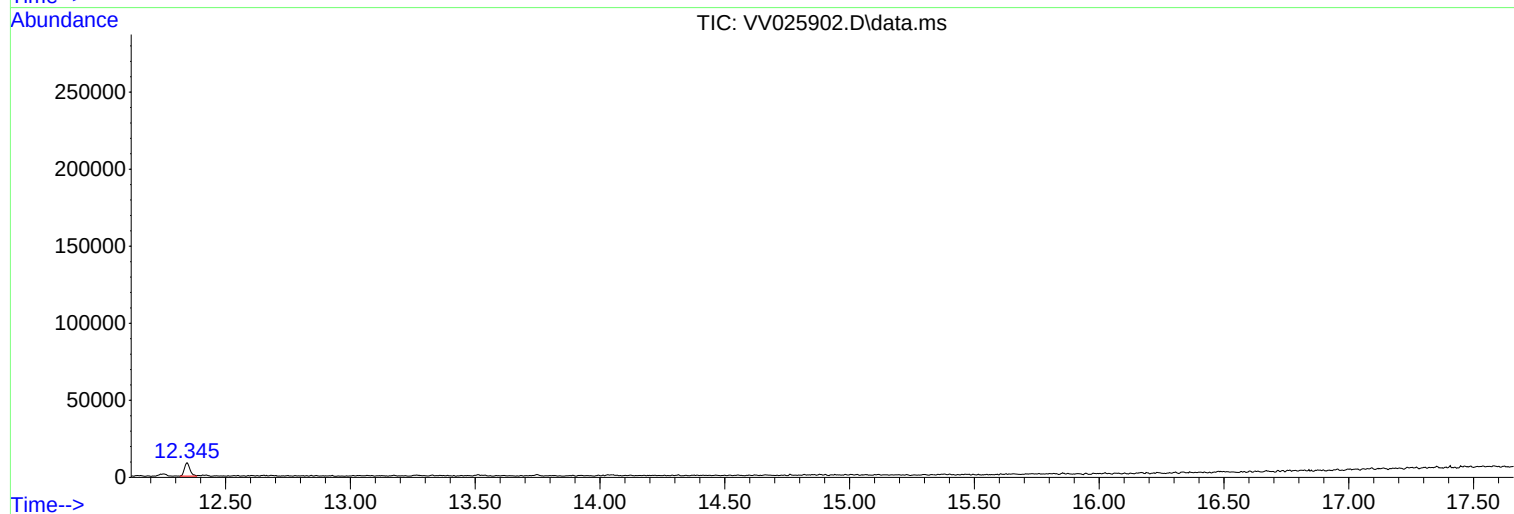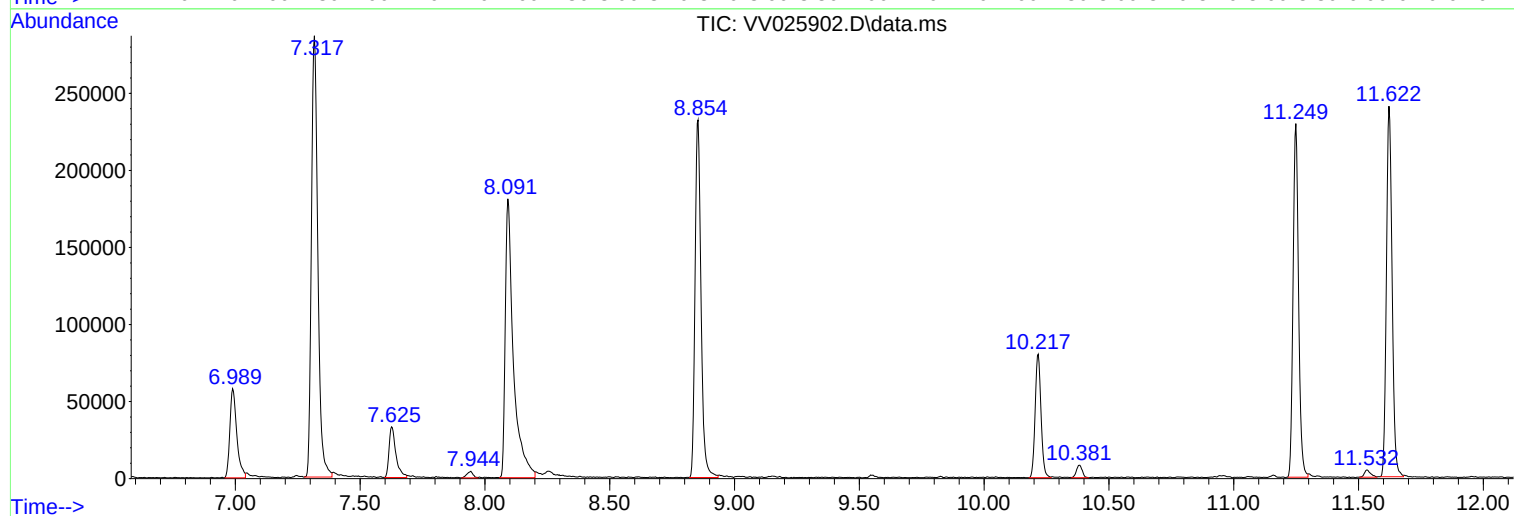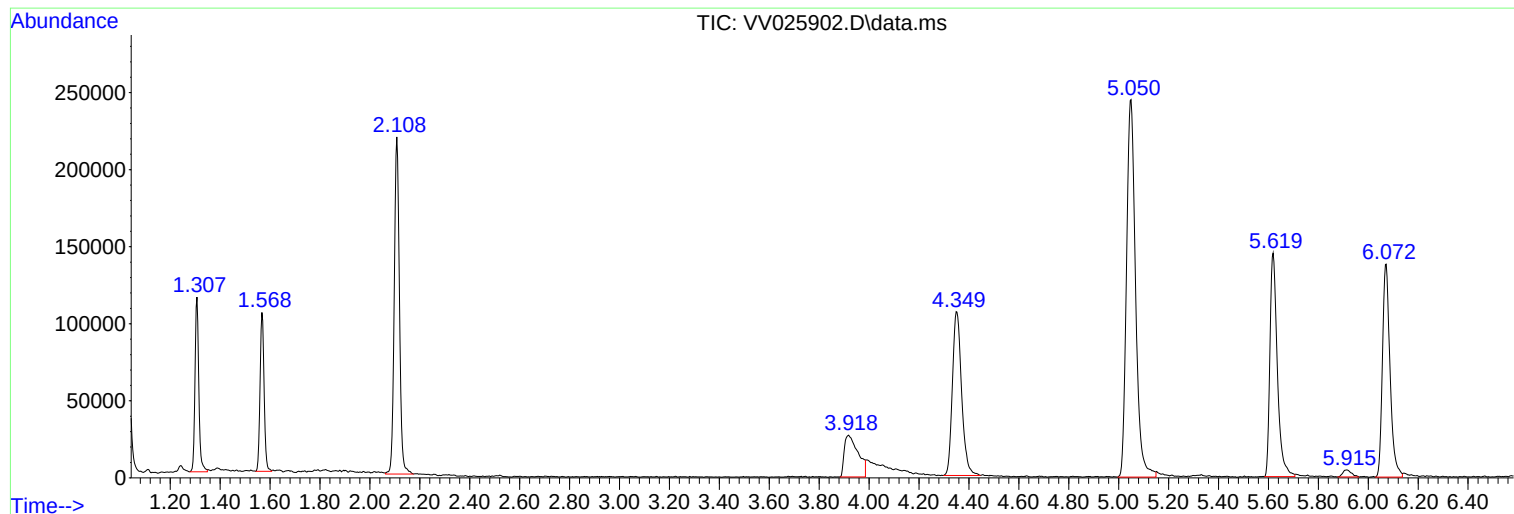

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051622\
Data File : VV025902.D
Acq On : 16 May 2022 11:15
Operator : SY/MD
Sample : N2831-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2L7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051622\
Data File : VV025902.D
Acq On : 16 May 2022 11:15
Operator : SY/MD
Sample : N2831-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2L7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc