

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051622\
 Data File : VV025914.D
 Acq On : 16 May 2022 16:03
 Operator : SY/MD
 Sample : N2831-01DL 20X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YB2J8DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025914.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	98	rVB	113056	115874	17.97%	2.007%
2	1.571	157	165	175	rBV	105435	122874	19.06%	2.128%
3	2.108	323	332	352	rVB2	238312	367211	56.95%	6.360%
4	2.510	447	457	475	rVB2	22728	39830	6.18%	0.690%
5	3.915	879	894	935	rBV3	49459	219643	34.07%	3.804%
6	4.352	1011	1030	1061	rBV	117317	294623	45.70%	5.103%
7	5.050	1231	1247	1283	rBV2	259421	644752	100.00%	11.167%
8	5.619	1412	1424	1450	rBV	213508	440657	68.35%	7.632%
9	5.915	1504	1516	1548	rBV	186375	380487	59.01%	6.590%
10	6.069	1552	1564	1587	rBV	146176	307601	47.71%	5.327%
11	6.989	1840	1850	1885	rBV	51228	104196	16.16%	1.805%
12	7.317	1941	1952	1985	rBV	297750	536183	83.16%	9.286%
13	7.625	2038	2048	2071	rBV2	29015	56874	8.82%	0.985%
14	7.976	2148	2157	2181	rVB2	24084	44628	6.92%	0.773%
15	8.091	2183	2193	2237	rBV	212596	443484	68.78%	7.681%
16	8.850	2418	2429	2447	rBV	347198	573927	89.02%	9.940%
17	10.217	2841	2854	2878	rBV	92560	149223	23.14%	2.584%
18	11.249	3162	3175	3197	rBV	342183	529403	82.11%	9.169%
19	11.622	3279	3291	3310	rBV	251802	402387	62.41%	6.969%




Sum of corrected areas: 5773857

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051622\
Data File : VV025914.D
Acq On : 16 May 2022 16:03
Operator : SY/MD
Sample : N2831-01DL 20X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2J8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

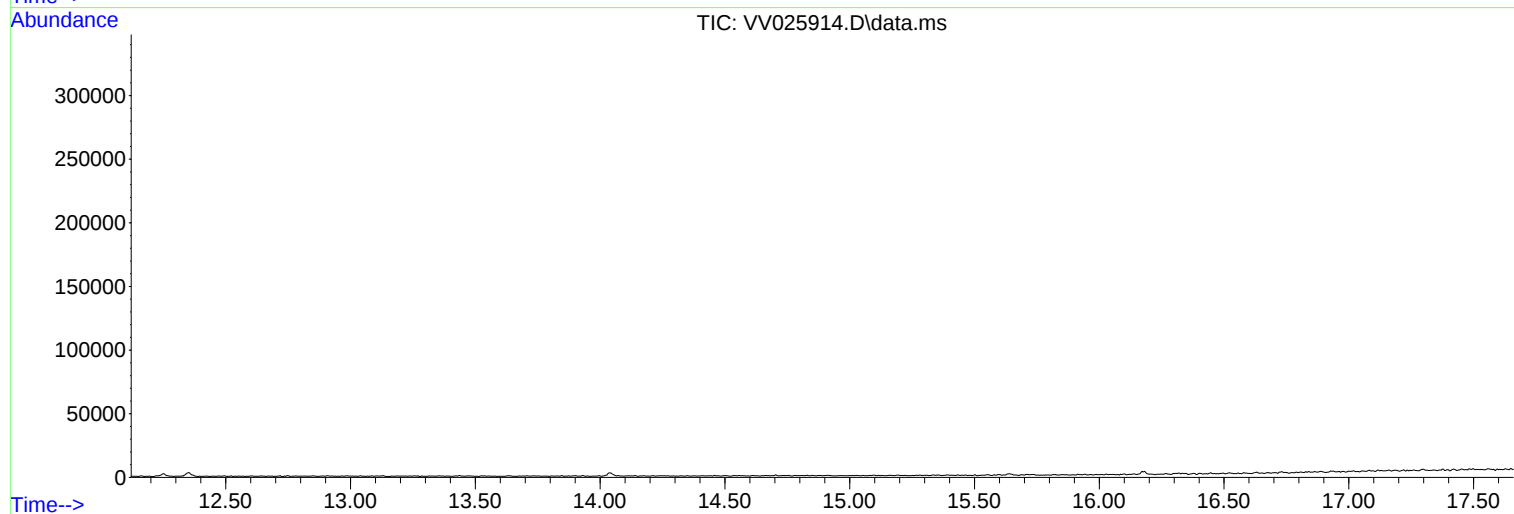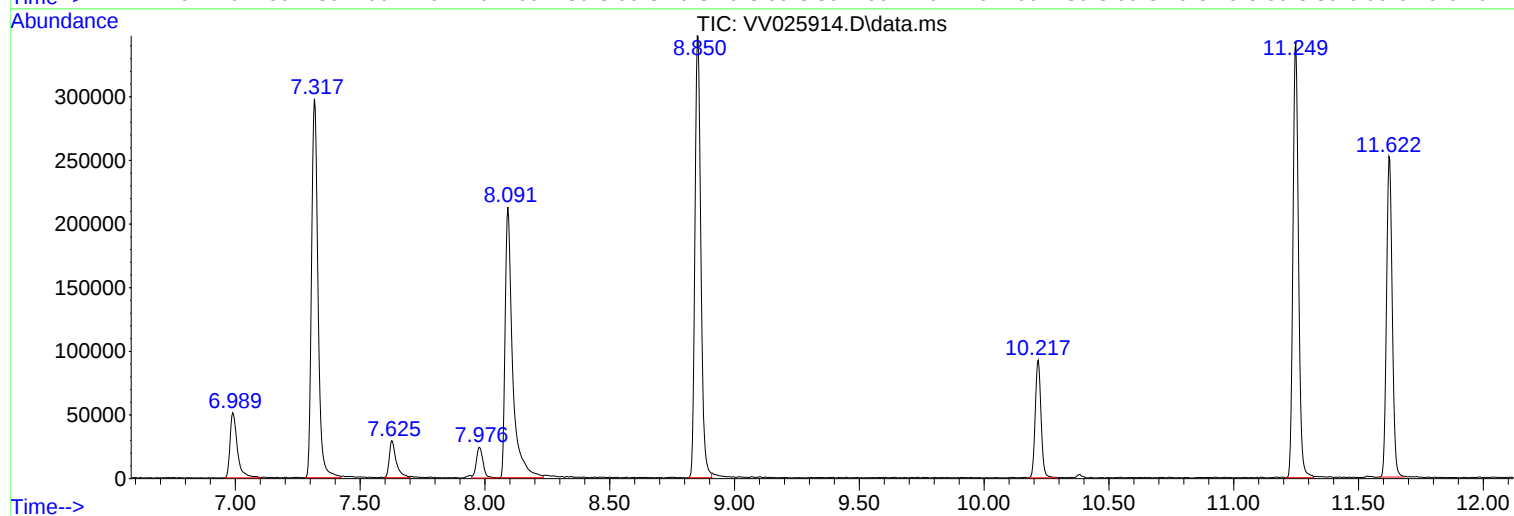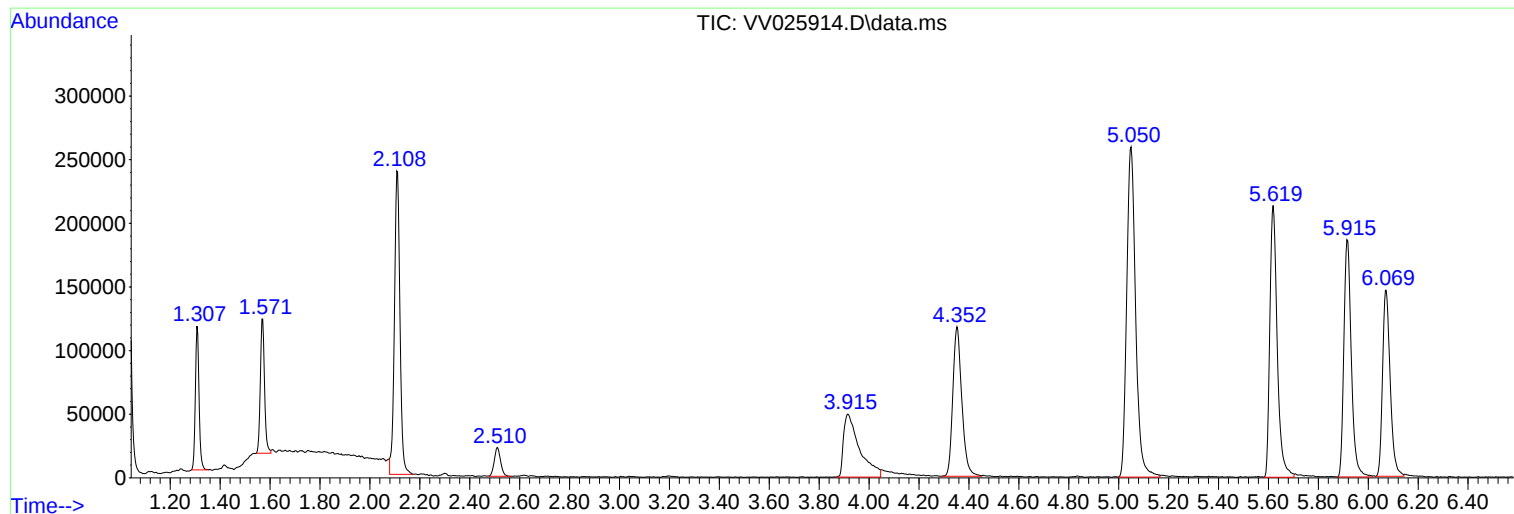

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051622\
Data File : VV025914.D
Acq On : 16 May 2022 16:03
Operator : SY/MD
Sample : N2831-01DL 20X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2J8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051622\
Data File : VV025914.D
Acq On : 16 May 2022 16:03
Operator : SY/MD
Sample : N2831-01DL 20X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2J8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc