

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051622\
 Data File : VV025915.D
 Acq On : 16 May 2022 16:27
 Operator : SY/MD
 Sample : N2831-03DL 20X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YB2K0DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025915.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	96	rBV	91548	103762	19.18%	2.185%
2	1.568	157	164	174	rBV	83533	101265	18.71%	2.133%
3	2.108	322	332	353	rVB3	215679	351067	64.88%	7.394%
4	2.506	446	456	467	rBV2	14340	24691	4.56%	0.520%
5	2.625	481	493	502	rBV3	4071	8618	1.59%	0.182%
6	3.915	879	894	929	rBV3	157689	474969	87.78%	10.003%
7	4.352	1013	1030	1057	rBV	94929	240663	44.48%	5.069%
8	5.050	1228	1247	1277	rBV2	217854	541093	100.00%	11.396%
9	5.619	1412	1424	1453	rBV	179456	370629	68.50%	7.806%
10	5.924	1506	1519	1537	rBV3	11690	26580	4.91%	0.560%
11	6.069	1551	1564	1585	rBV	119234	251714	46.52%	5.301%
12	6.992	1840	1851	1874	rBV2	38560	78734	14.55%	1.658%
13	7.317	1941	1952	1976	rBV	241244	434681	80.33%	9.155%
14	7.628	2041	2049	2066	rBV2	20136	38723	7.16%	0.816%
15	8.091	2182	2193	2234	rBV	170518	356415	65.87%	7.507%
16	8.853	2418	2430	2450	rBV	283914	470974	87.04%	9.919%
17	10.217	2843	2854	2868	rBV2	74576	118688	21.93%	2.500%
18	11.249	3164	3175	3194	rBV	272563	430279	79.52%	9.062%
19	11.622	3280	3291	3306	rBV	203463	324523	59.98%	6.835%




Sum of corrected areas: 4748068

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051622\
Data File : VV025915.D
Acq On : 16 May 2022 16:27
Operator : SY/MD
Sample : N2831-03DL 20X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2K0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

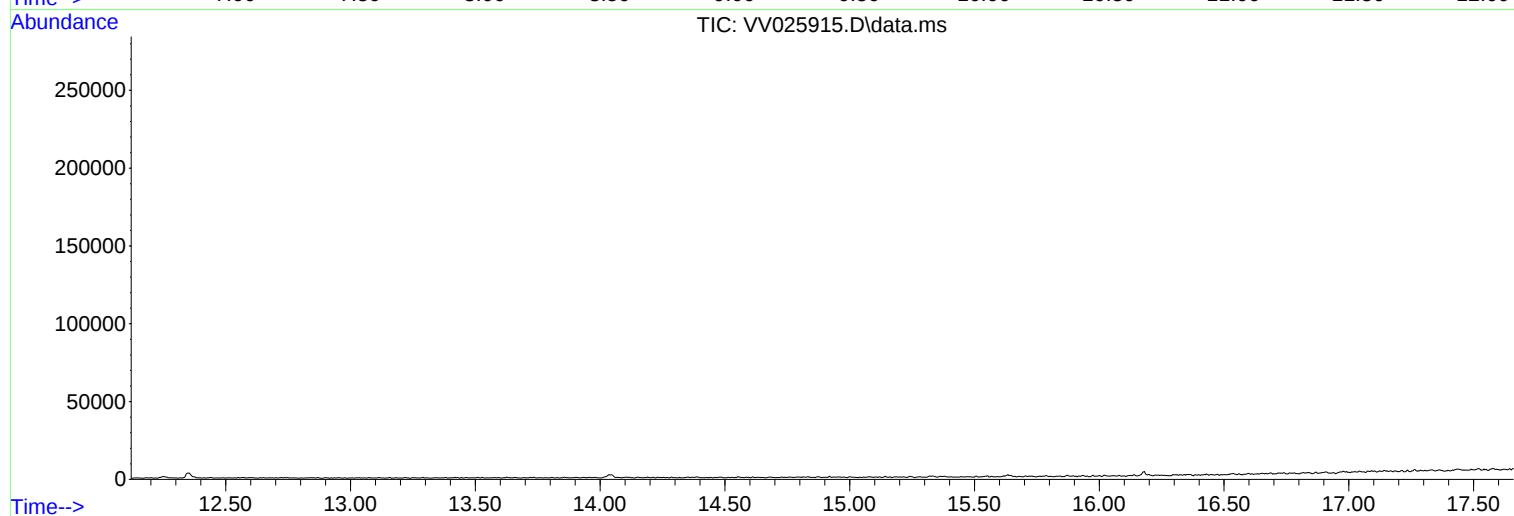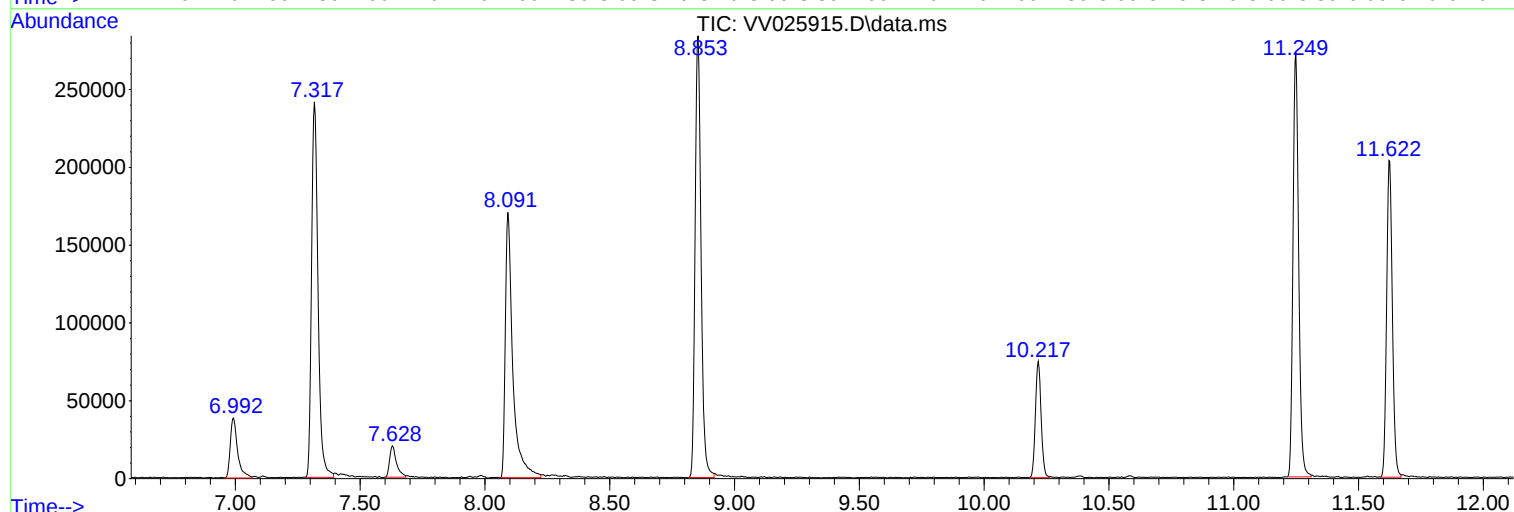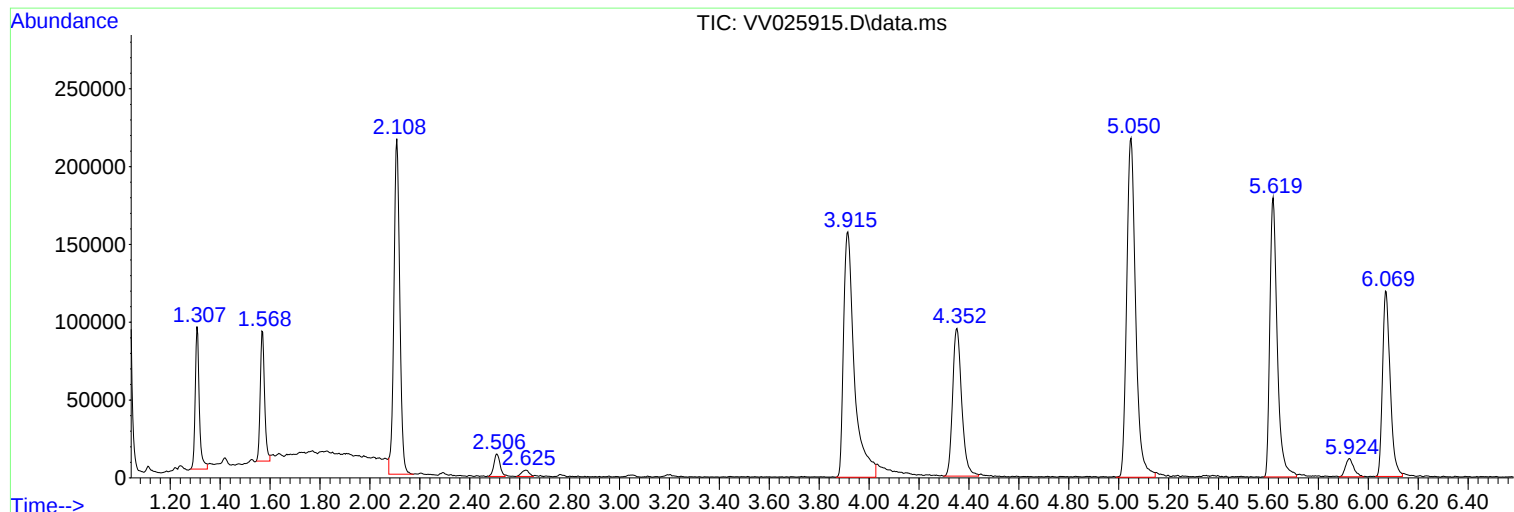

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051622\
Data File : VV025915.D
Acq On : 16 May 2022 16:27
Operator : SY/MD
Sample : N2831-03DL 20X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2K0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051622\
Data File : VV025915.D
Acq On : 16 May 2022 16:27
Operator : SY/MD
Sample : N2831-03DL 20X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YB2K0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
