
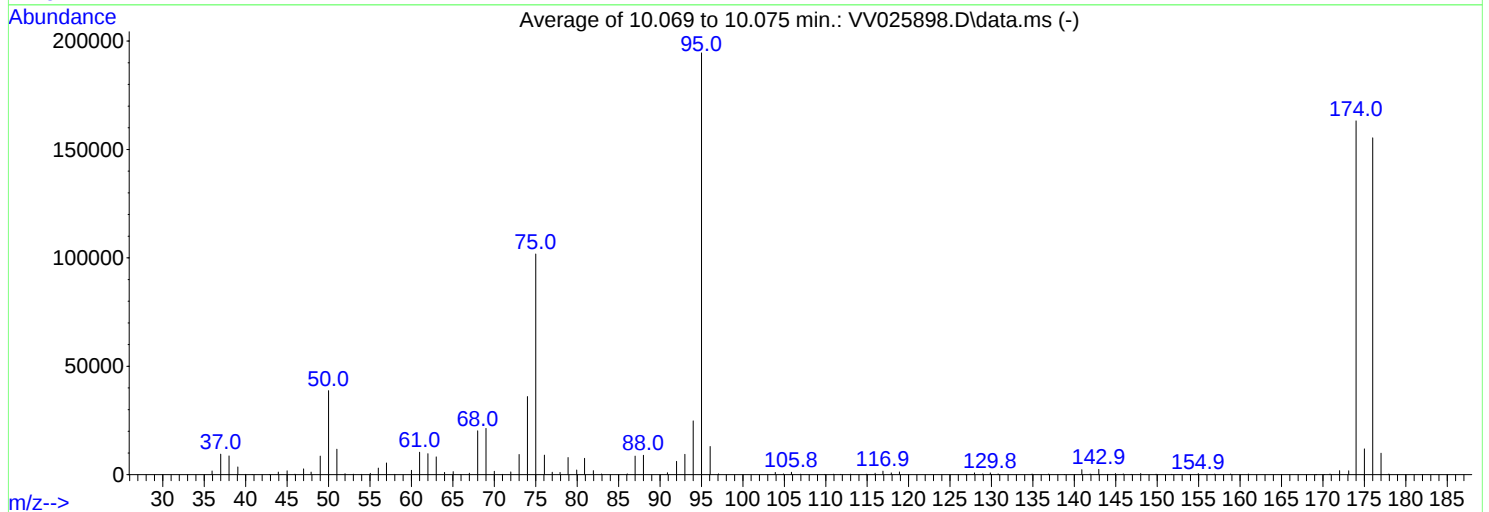


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051622\
 Data File : VV025898.D
 Acq On : 16 May 2022 09:16
 Operator : SY/MD
 Sample : BFB317
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB317

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR051322WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed May 18 05:55:49 2022

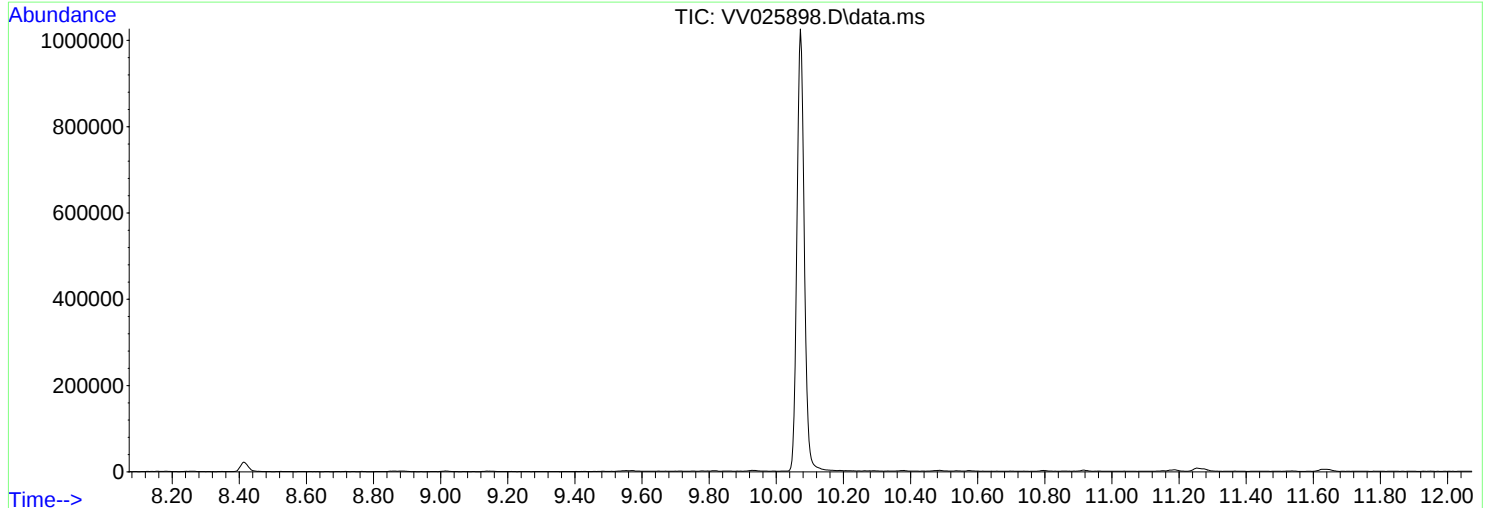

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	38728	PASS
75	95	30	80	52.3	101752	PASS
95	95	100	100	100.0	194560	PASS
96	95	5	9	6.7	13010	PASS
173	174	0.00	2	1.1	1769	PASS
174	95	50	120	83.9	163179	PASS
175	174	5	9	7.3	11853	PASS
176	174	95	105	95.2	155392	PASS
177	176	5	10	6.4	9923	PASS

Scan 2795 (10.027 min): VV025898.D\data.ms
BFB317

m/z	Abundance
35.90	747.0
38.00	397.0
40.00	233.0
44.00	417.0

Instrument :
MSVOA_V
ClientSampleId :
BFB317

m/z	Abundance
36.00	2418.0
37.00	9272.0
38.00	9299.0
39.00	3732.0
40.10	477.0
40.80	103.0
42.80	105.0
43.90	1602.0
45.00	1799.0
46.00	230.0
47.00	2685.0
47.90	1195.0
49.00	8877.0
50.00	38424.0
51.00	11864.0
52.00	446.0
53.00	275.0
53.90	126.0
55.10	634.0
56.00	2989.0
57.00	5601.0
57.90	181.0
60.00	1908.0
61.00	10396.0
62.00	9992.0
63.00	8561.0
64.00	1200.0
65.00	1356.0
67.00	652.0
68.00	20448.0
69.00	20920.0
70.00	1573.0
70.90	122.0
72.00	1200.0
73.00	9062.0
74.00	35536.0
75.00	99616.0
76.00	8964.0
77.00	1212.0
77.90	1125.0
78.90	7968.0
79.90	2069.0
80.90	7451.0
82.00	1807.0
82.90	288.0
86.00	331.0
87.00	8486.0
88.00	8538.0
90.90	820.0
92.00	5694.0
93.00	9394.0
94.00	24288.0
95.00	191680.0
96.10	13269.0
97.10	406.0
103.90	1019.0
104.90	370.0
105.90	1131.0
106.90	214.0
109.90	140.0
110.90	229.0
111.80	125.0
113.00	195.0
114.90	202.0
115.90	632.0
116.90	1487.0
117.90	863.0
118.90	1288.0
127.90	856.0
128.90	428.0
129.80	755.0
130.80	328.0
134.90	326.0
136.90	301.0
138.80	106.0
140.90	2093.0
141.90	341.0
143.00	2433.0
144.00	189.0
144.90	506.0
145.90	350.0
146.80	155.0
148.00	482.0
149.80	260.0
151.80	165.0
152.80	158.0
153.90	149.0
155.00	556.0
155.80	122.0
157.00	276.0
158.90	219.0
161.00	313.0

Instrument :
MSVOA_V
ClientSampleId :
BFB317

170.10	105.0
170.90	334.0
172.00	1912.0
173.10	1688.0
174.00	156672.0
175.00	11621.0
176.00	149056.0
177.00	9762.0
177.90	348.0

Instrument :
MSVOA_V
ClientSampleId :
BFB317

m/z	Abundance
36.00	2515.0
37.00	9800.0
38.00	9380.0
39.00	3644.0
40.10	439.0
40.80	103.0
42.90	112.0
43.90	1657.0
45.00	1815.0
45.90	241.0
47.00	2829.0
47.90	1287.0
49.00	8952.0
50.00	40176.0
51.00	12026.0
52.00	456.0
53.00	251.0
53.90	135.0
55.00	657.0
56.00	3093.0
57.00	5572.0
58.00	169.0
60.00	2061.0
61.00	10751.0
62.00	10067.0
63.00	8395.0
64.00	1083.0
65.00	1465.0
65.90	179.0
67.00	709.0
68.00	20872.0
69.00	22112.0
70.00	1584.0
71.00	136.0
72.00	1341.0
73.00	9649.0
74.00	37352.0
75.00	105576.0
76.10	9333.0
77.00	1101.0
77.90	1094.0
78.90	8171.0
79.90	2195.0
80.90	7825.0
81.90	1884.0
83.00	277.0
86.10	332.0
87.00	8835.0
88.00	9404.0
90.90	888.0
92.00	6406.0
93.00	9712.0
94.00	25720.0
95.00	201472.0
96.10	13528.0
97.10	337.0
103.90	1084.0
104.90	360.0
105.80	1166.0
107.00	253.0
109.90	142.0
110.90	230.0
111.80	167.0
113.00	233.0
114.90	202.0
116.00	732.0
116.90	1651.0
117.90	854.0
118.90	1380.0
128.00	819.0
128.90	405.0
129.90	865.0
130.80	375.0
134.90	327.0
136.90	334.0
138.80	111.0
140.10	184.0
140.90	2407.0
141.90	339.0
142.90	2536.0
144.10	187.0
145.00	505.0
145.90	350.0
146.80	163.0
148.00	523.0
149.80	242.0
151.70	155.0
152.80	131.0
154.00	157.0
155.00	580.0
157.00	312.0
158.80	293.0

Instrument :
MSVOA_V
ClientSampleId :
BFB317

161.00	296.0
170.20	111.0
170.80	324.0
172.00	1885.0
173.10	1774.0
174.00	169600.0
175.00	12366.0
176.00	161408.0
177.00	10329.0
178.00	331.0

Instrument :
MSVOA_V
ClientSampleId :
BFB317

m/z	Abundance
36.00	2409.0
37.00	9189.0
38.00	8399.0
39.10	3371.0
40.00	355.0
43.00	125.0
44.00	1574.0
45.00	1636.0
45.90	235.0
47.00	2502.0
47.90	1177.0
49.00	7990.0
50.00	37584.0
51.00	11401.0
52.00	447.0
53.00	221.0
54.00	127.0
55.00	567.0
56.00	2933.0
57.00	4948.0
58.10	174.0
60.00	1910.0
61.00	9967.0
62.00	8956.0
63.00	7566.0
64.00	908.0
65.10	1402.0
66.00	170.0
67.00	690.0
68.00	19264.0
69.00	20952.0
70.00	1507.0
71.10	106.0
72.00	1276.0
73.00	9276.0
74.00	35200.0
75.00	100064.0
76.00	8792.0
77.00	1029.0
78.00	982.0
78.90	7559.0
80.00	2109.0
80.90	7382.0
81.90	1817.0
83.00	242.0
86.10	368.0
87.00	8368.0
88.00	8903.0
90.90	860.0
92.00	6369.0
93.00	9014.0
94.00	24296.0
95.00	190528.0
96.00	12233.0
97.00	300.0
103.90	1070.0
104.90	295.0
105.80	1021.0
106.90	249.0
109.90	134.0
111.00	211.0
111.80	192.0
113.00	235.0
114.90	192.0
116.00	714.0
116.90	1690.0
117.90	804.0
118.90	1208.0
126.90	108.0
128.00	729.0
129.00	363.0
129.90	848.0
130.80	386.0
134.90	317.0
136.90	302.0
140.00	164.0
140.90	2342.0
141.90	308.0
142.90	2446.0
144.00	143.0
145.00	541.0
145.90	324.0
146.90	147.0
148.00	486.0
149.90	219.0
151.70	151.0
154.00	164.0
154.90	521.0
156.90	319.0
158.80	328.0
161.00	243.0
169.10	102.0

Instrument :
MSVOA_V
ClientSampleId :
BFB317

170.80	298.0
172.00	1716.0
173.10	1846.0
174.00	163264.0
175.00	11573.0
176.00	155712.0
177.00	9679.0
178.00	304.0

Instrument :
MSVOA_V
ClientSampleId :
BFB317