
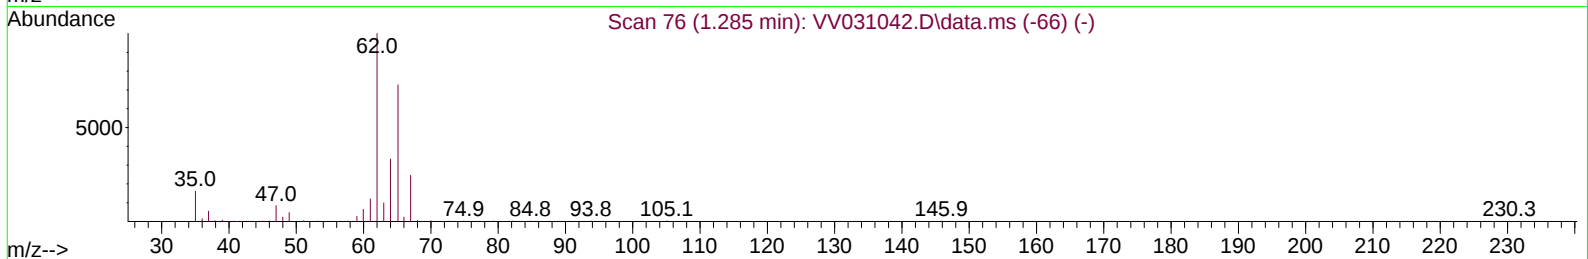
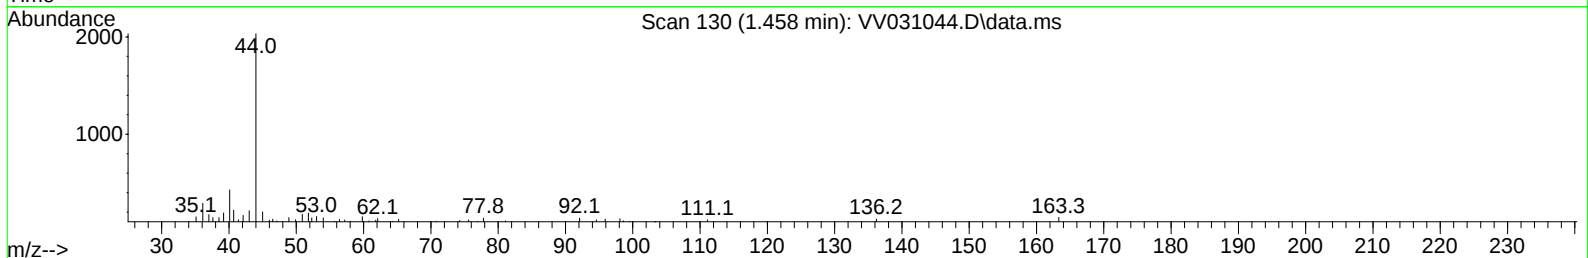


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051623\
 Data File : VV031044.D
 Acq On : 16 May 2023 11:41
 Operator : SY/MD
 Sample : 02790-03DL 250X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Quant Time: May 17 01:42:13 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed May 17 01:41:23 2023
 Response via : Initial Calibration

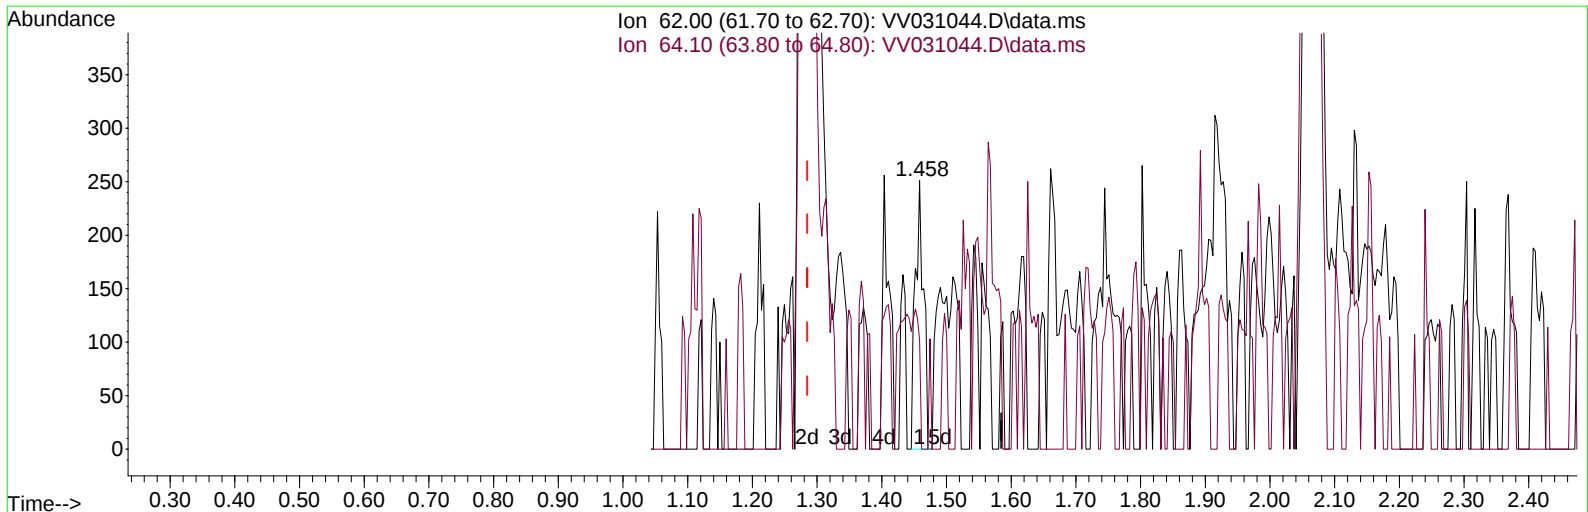

TIC: VV031044.D\data.ms

(5) Vinyl chloride (T)

1.458min (+ 0.173) 0.02 ug/L

response 220

Ion	Exp%	Act%
62.00	100.00	100.00
64.10	32.60	40.64
0.00	0.00	0.00
0.00	0.00	0.00