




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051623\
 Data File : VV031046.D
 Acq On : 16 May 2023 12:28
 Operator : SY/MD
 Sample : 02790-07DL 250X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CONY1DL

Manual IntegrationsAPPROVED

Quant Time: May 17 01:42:45 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed May 17 01:41:23 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/17/2023
 Supervised By :Mahesh Dadoda 05/17/2023

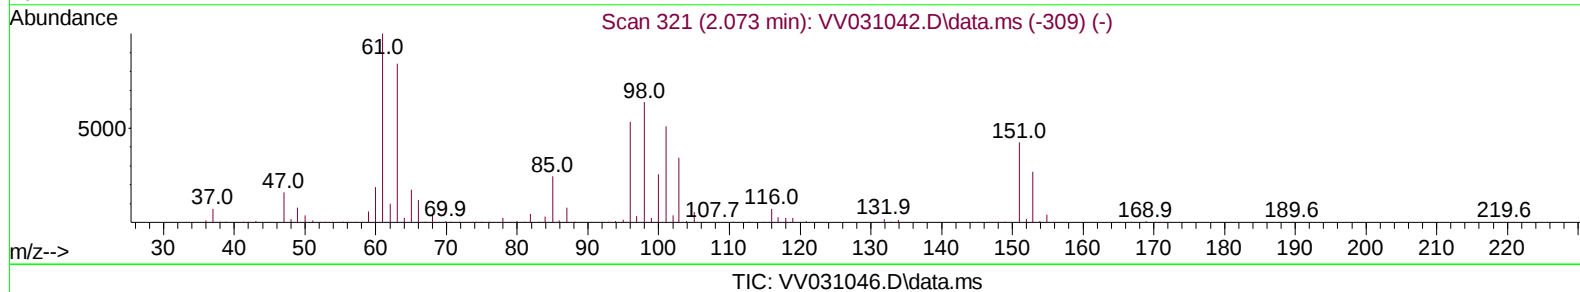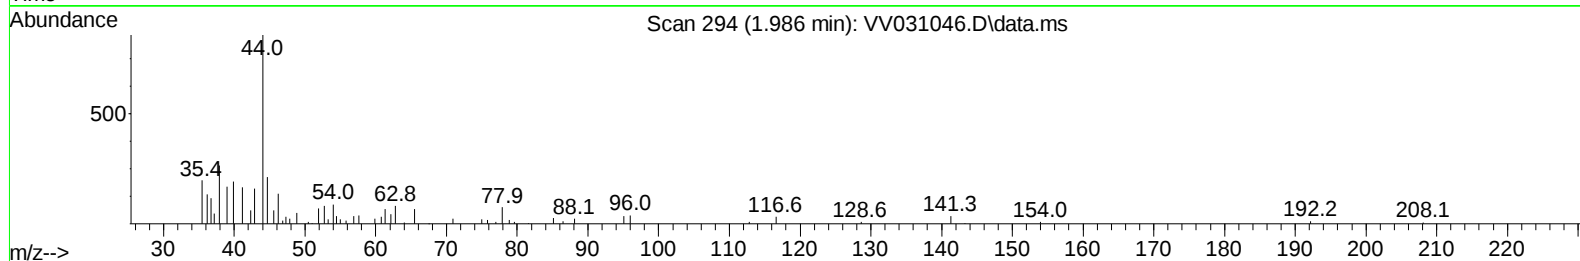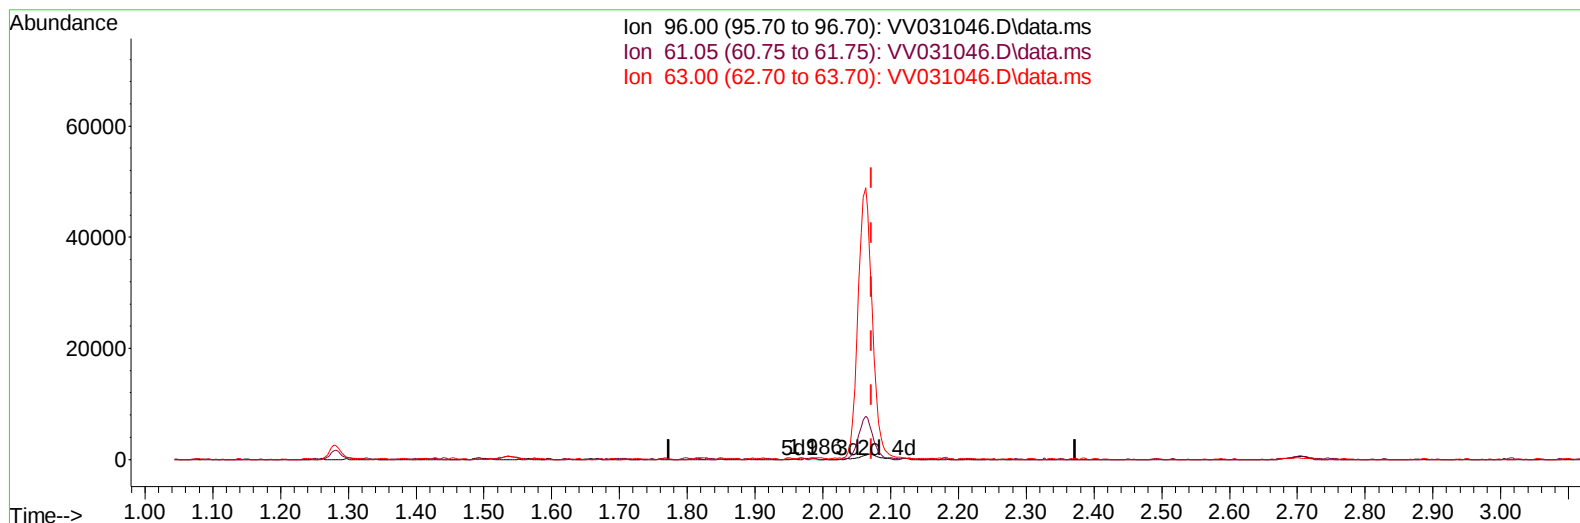

(12) 1,1-Dichloroethene (T)

1.986min (-0.087) 0.01 ug/L

response 70

Ion	Exp%	Act%
96.00	100.00	100.00
61.05	193.70	212.21
63.00	173.00	126.72
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051623\
 Data File : VV031046.D
 Acq On : 16 May 2023 12:28
 Operator : SY/MD
 Sample : 02790-07DL 250X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CONY1DL

Manual IntegrationsAPPROVED

Quant Time: May 17 01:42:45 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed May 17 01:41:23 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/17/2023
 Supervised By :Mahesh Dadoda 05/17/2023

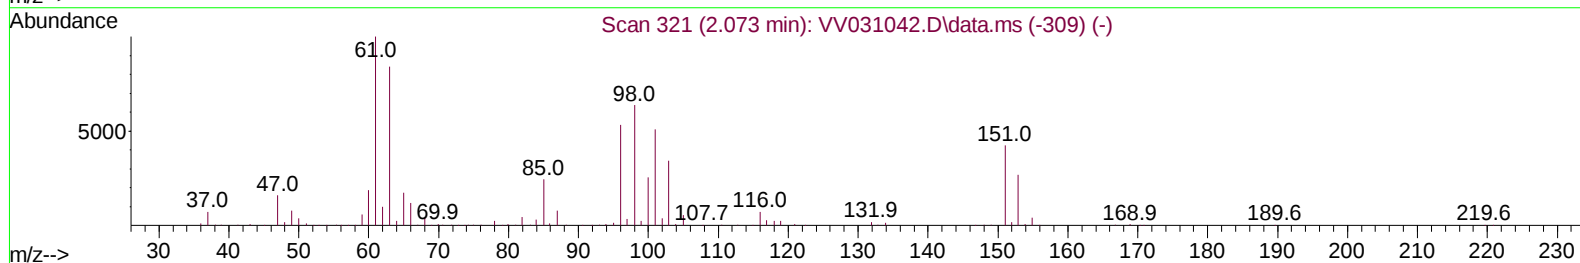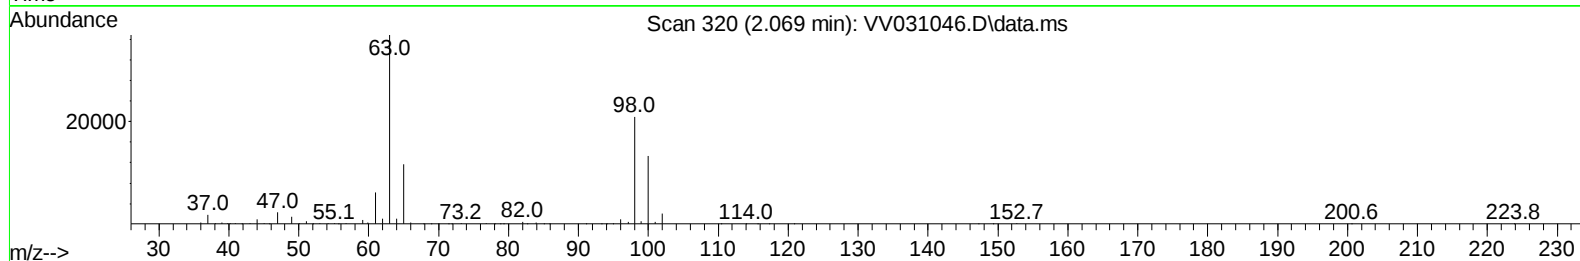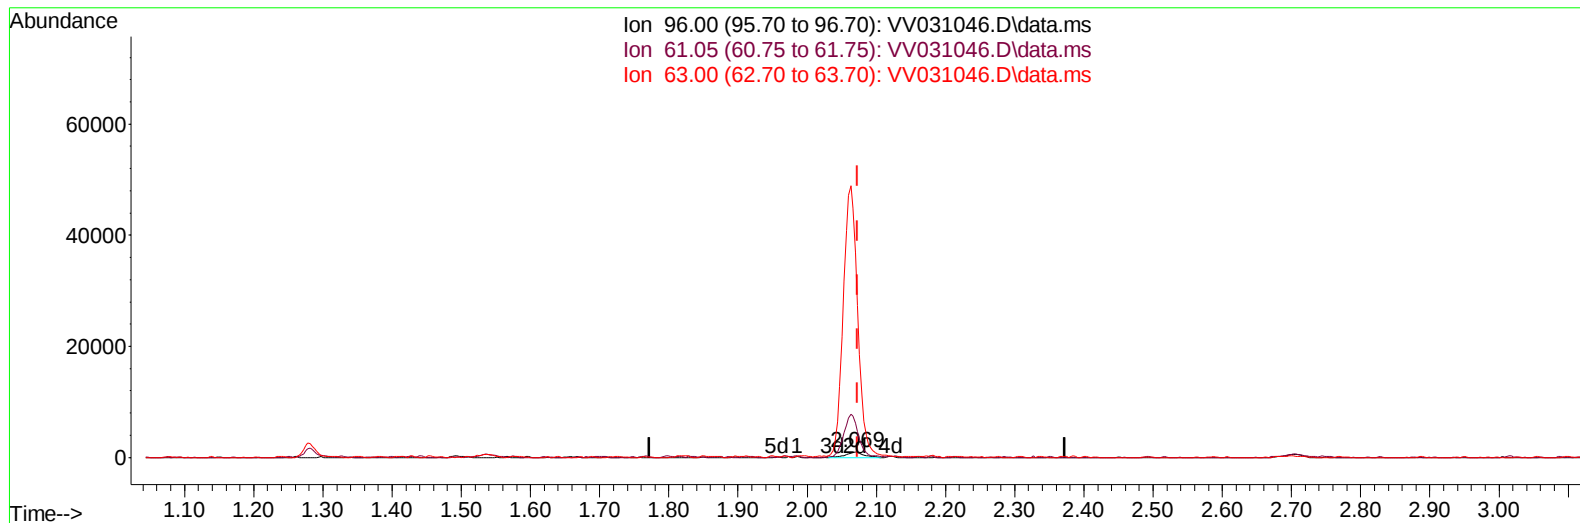

TIC: VV031046.D\data.ms

(12) 1,1-Dichloroethene (T)

2.069min (-0.003) 0.19 ug/L m

response 1765

Ion	Exp%	Act%
96.00	100.00	100.00
61.05	193.70	633.40#
63.00	173.00	3763.02#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051623\
 Data File : VV031046.D
 Acq On : 16 May 2023 12:28
 Operator : SY/MD
 Sample : 02790-07DL 250X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CONY1DL

Manual IntegrationsAPPROVED

Quant Time: May 17 01:42:45 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed May 17 01:41:23 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/17/2023
 Supervised By :Mahesh Dadoda 05/17/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	137511	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.793	117	136385	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	69910	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	40875	3.608	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	72.200%		
7) Chloroethane-d5	1.536	69	38562	4.172	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	83.400%		
11) 1,1-Dichloroethene-d2	2.063	65	22927	3.824	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	76.400%		
20) 2-Butanone-d5	3.844	46	86966	43.287	ug/L	0.02
Spiked Amount 50.000	Range 40 - 130		Recovery =	86.580%		
24) Chloroform-d	4.259	84	98585	4.378	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	87.600%		
26) 1,2-Dichloroethane-d4	4.953	65	51516	4.500	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	90.000%		
32) Benzene-d6	4.970	84	168009	4.203	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	84.000%		
36) 1,2-Dichloropropane-d6	5.998	67	49258	4.237	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	84.800%		
41) Toluene-d8	7.249	98	139302	3.659	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	73.200%		
43) trans-1,3-Dichloroprop...	7.564	79	17103	3.925	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	78.400%		
46) 2-Hexanone-d5	8.037	63	58856	38.551	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	77.100%		
56) 1,1,2,2-Tetrachloroeth...	10.162	84	35563	4.221	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	84.400%		
66) 1,2-Dichlorobenzene-d4	11.567	152	54453	4.178	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	83.600%		
Target Compounds						
						Qvalue
5) Vinyl chloride	1.285	62	5022	0.471	ug/L	90
12) 1,1-Dichloroethene	2.069	96	1765m	0.191	ug/L	
16) Methylene chloride	2.455	84	6423	0.614	ug/L	88
18) trans-1,2-Dichloroethene	2.706	96	957	0.113	ug/L	83
22) cis-1,2-Dichloroethene	3.825	96	28503	3.196	ug/L	98
34) Trichloroethene	5.841	95	98468	10.768	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051623\
Data File : VV031046.D
Acq On : 16 May 2023 12:28
Operator : SY/MD
Sample : 02790-07DL 250X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CONY1DL

Manual IntegrationsAPPROVED

Quant Time: May 17 01:42:45 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed May 17 01:41:23 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 05/17/2023
Supervised By :Mahesh Dadoda 05/17/2023

