

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051623\
 Data File : VV031048.D
 Acq On : 16 May 2023 13:18
 Operator : SY/MD
 Sample : 02767-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C11F0

Quant Time: May 17 01:43:18 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed May 17 01:41:23 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	123382	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	122917	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	60333	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	38832	3.820	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	76.400%
7) Chloroethane-d5	1.536	69	39856	4.806	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.200%
11) 1,1-Dichloroethene-d2	2.063	65	22141	4.116	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	82.400%
20) 2-Butanone-d5	3.815	46	89686	49.753	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	99.500%
24) Chloroform-d	4.259	84	99302	4.915	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.400%
26) 1,2-Dichloroethane-d4	4.953	65	53611	5.220	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.400%
32) Benzene-d6	4.970	84	167907	4.660	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.200%
36) 1,2-Dichloropropane-d6	5.998	67	50614	4.831	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.600%
41) Toluene-d8	7.252	98	141916	4.136	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.800%
43) trans-1,3-Dichloroprop...	7.564	79	16498	4.201	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.000%
46) 2-Hexanone-d5	8.034	63	62346	45.312	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	90.620%
56) 1,1,2,2-Tetrachloroeth...	10.159	84	36883	4.857	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.200%
66) 1,2-Dichlorobenzene-d4	11.571	152	57626	5.124	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.400%
Target Compounds						
13) Acetone	2.156	43	4209	2.733	ug/L	Qvalue 66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051623\
Data File : VV031048.D
Acq On : 16 May 2023 13:18
Operator : SY/MD
Sample : 02767-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C11F0

Quant Time: May 17 01:43:18 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed May 17 01:41:23 2023
Response via : Initial Calibration

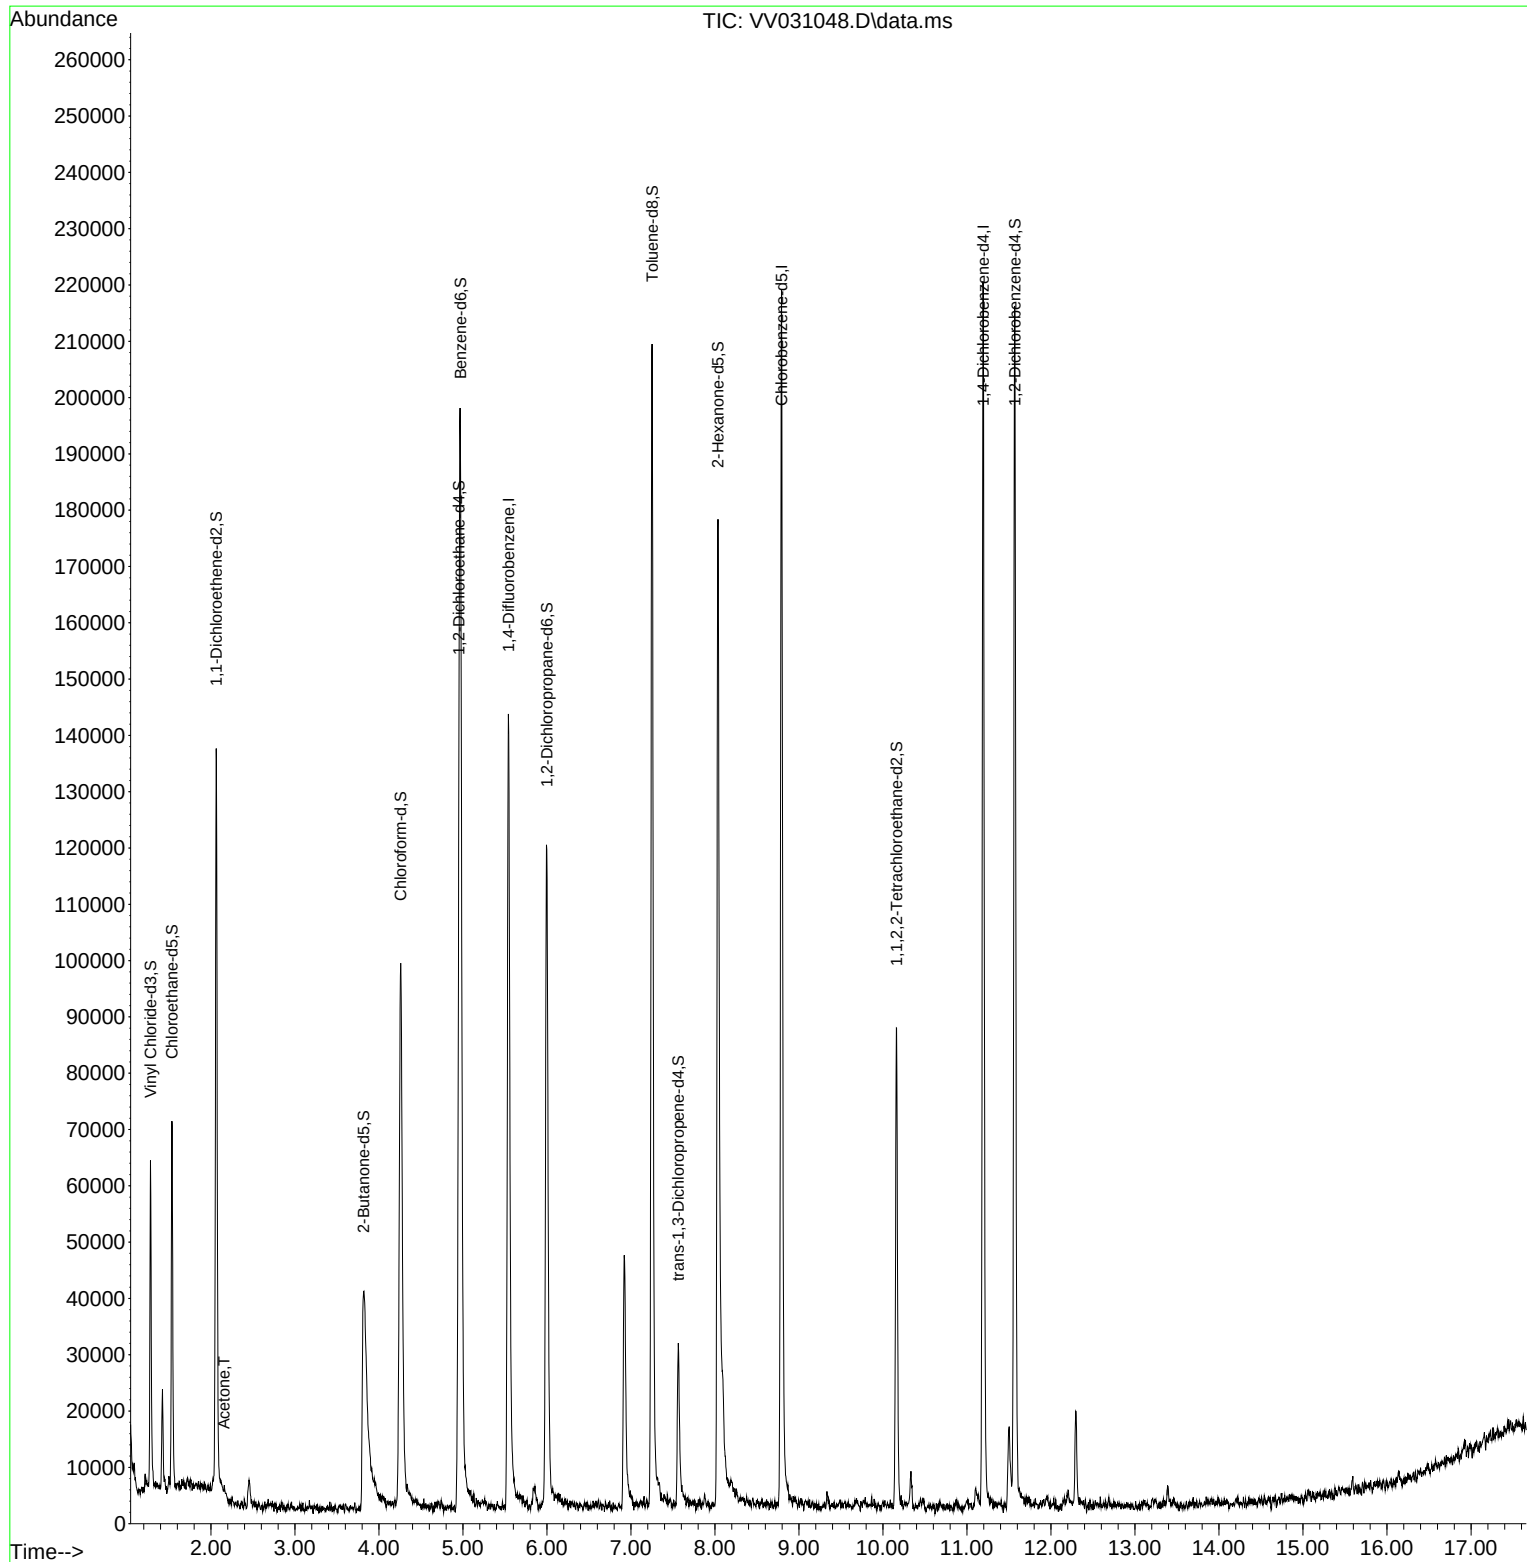

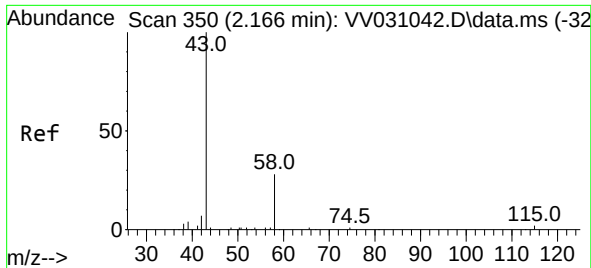

#13
 Acetone
 Concen: 2.733 ug/L
 RT: 2.156 min Scan# 34
 Delta R.T. -0.010 min
 Lab File: VV031048.D
 Acq: 16 May 2023 13:18

Instrument :
 MSVOA_V
 ClientSampleId :
 C11F0

Tgt Ion: 43 Resp: 4209
 Ion Ratio Lower Upper
 43 100
 58 3.3 0.0 37.0

