

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW051623\
 Data File : VW031057.D
 Acq On : 16 May 2023 16:50
 Operator : SY/MD
 Sample : 02768-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CONP5

Quant Time: May 17 01:45:36 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed May 17 01:41:23 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	120443	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.793	117	119314	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.191	152	63011	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	36482	3.676	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	73.600%	
7) Chloroethane-d5	1.539	69	37862	4.677	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	93.600%	
11) 1,1-Dichloroethene-d2	2.063	65	21076	4.013	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	80.200%	
20) 2-Butanone-d5	3.818	46	100851	57.312	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	114.620%	
24) Chloroform-d	4.259	84	92949	4.713	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	94.200%	
26) 1,2-Dichloroethane-d4	4.953	65	53729	5.359	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	107.200%	
32) Benzene-d6	4.970	84	155710	4.452	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	89.000%	
36) 1,2-Dichloropropane-d6	5.998	67	48032	4.723	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	94.400%	
41) Toluene-d8	7.252	98	129026	3.874	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	77.400%	
43) trans-1,3-Dichloroprop...	7.561	79	15803	4.145	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	83.000%	
46) 2-Hexanone-d5	8.034	63	73439	54.986	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	109.980%	
56) 1,1,2,2-Tetrachloroeth...	10.159	84	38996	5.290	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	105.800%	
66) 1,2-Dichlorobenzene-d4	11.571	152	53911	4.590	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	91.800%	
Target Compounds						
					Qvalue	
13) Acetone	2.143	43	3342	2.223	ug/L	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051623\
Data File : VV031057.D
Acq On : 16 May 2023 16:50
Operator : SY/MD
Sample : 02768-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CONP5

Quant Time: May 17 01:45:36 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed May 17 01:41:23 2023
Response via : Initial Calibration

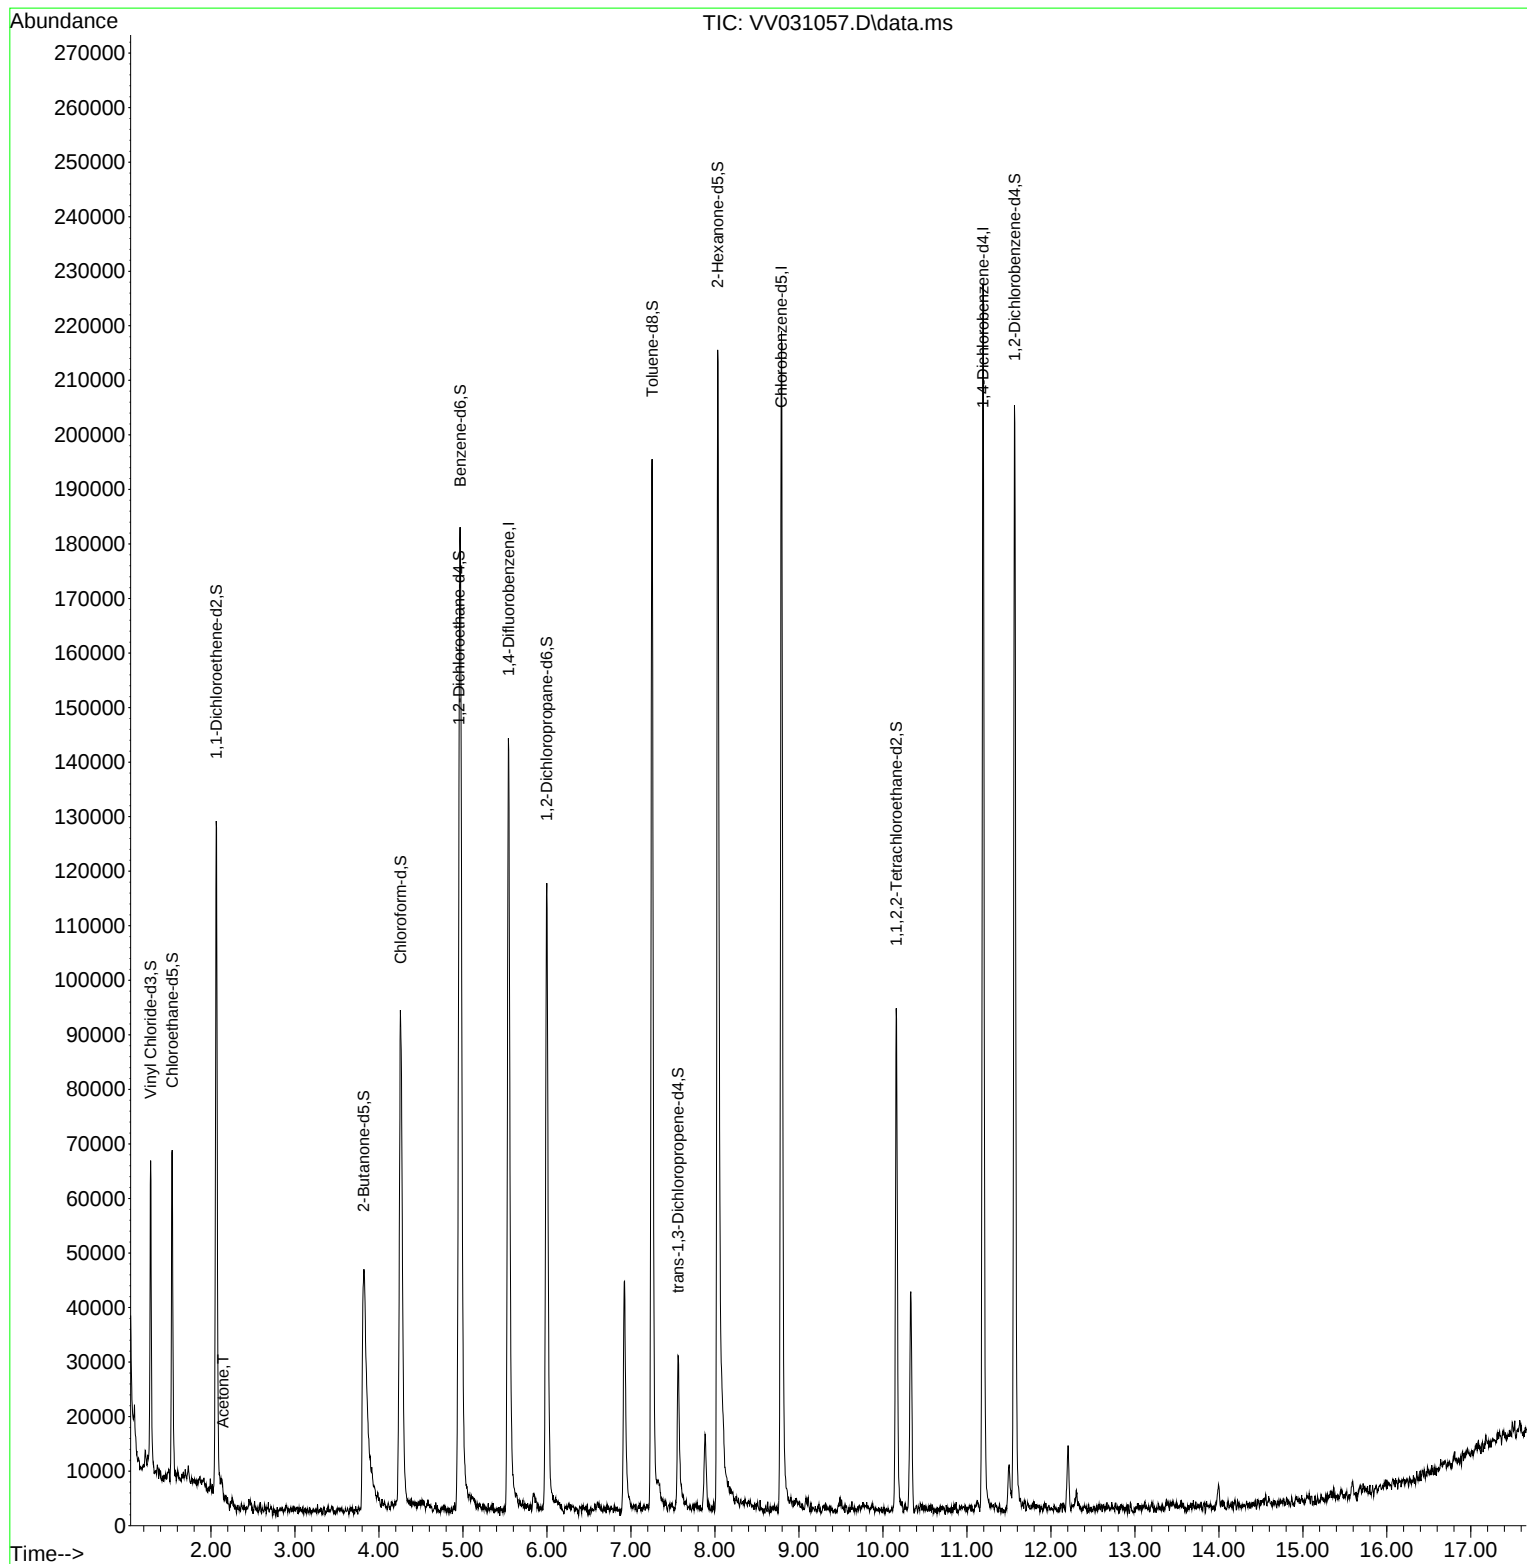

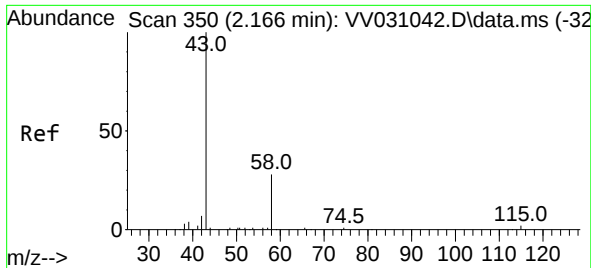

#13
Acetone
Concen: 2.223 ug/L
RT: 2.143 min Scan# 34
Delta R.T. -0.023 min
Lab File: VV031057.D
Acq: 16 May 2023 16:50

Instrument :
MSVOA_V
ClientSampleId :
CONP5

Tgt Ion: 43 Resp: 3342
Ion Ratio Lower Upper
43 100
58 10.7 0.0 37.0

