

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051623\
 Data File : VV031044.D
 Acq On : 16 May 2023 11:41
 Operator : SY/MD
 Sample : 02790-03DL 250X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CONX7DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV031044.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	84	rBV2	64296	72734	10.90%	1.517%
2	1.536	147	154	168	rVB	62230	74024	11.10%	1.544%
3	2.063	308	318	329	rBV	131489	191309	28.68%	3.990%
4	2.146	342	344	358	rVB	6352	8831	1.32%	0.184%
5	2.455	432	440	453	rVB2	8130	15484	2.32%	0.323%
6	3.828	851	867	892	rBV4	71892	247038	37.03%	5.152%
7	4.259	978	1001	1018	rBV	91050	236962	35.52%	4.942%
8	4.966	1205	1221	1249	rBV3	179842	472307	70.80%	9.850%
9	5.542	1388	1400	1423	rBV	171660	364277	54.61%	7.597%
10	5.838	1478	1492	1511	rBV	328719	667088	100.00%	13.913%
11	5.995	1529	1541	1557	rBV	111574	231714	34.74%	4.833%
12	6.921	1817	1829	1844	rBV2	43857	89831	13.47%	1.873%
13	7.249	1920	1931	1951	rBV	194886	355768	53.33%	7.420%
14	7.561	2020	2028	2042	rBV2	26540	51389	7.70%	1.072%
15	8.040	2164	2177	2207	rBV	144345	366098	54.88%	7.635%
16	8.792	2397	2411	2435	rBV	269313	462951	69.40%	9.655%
17	10.162	2826	2837	2854	rBV	79785	130813	19.61%	2.728%
18	11.191	3147	3157	3174	rBV	262240	428877	64.29%	8.945%
19	11.567	3263	3274	3289	rBV	195248	318820	47.79%	6.649%
20	12.201	3462	3471	3480	rBV8	5286	8513	1.28%	0.178%




Sum of corrected areas: 4794828

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051623\
Data File : VV031044.D
Acq On : 16 May 2023 11:41
Operator : SY/MD
Sample : 02790-03DL 250X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CONX7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

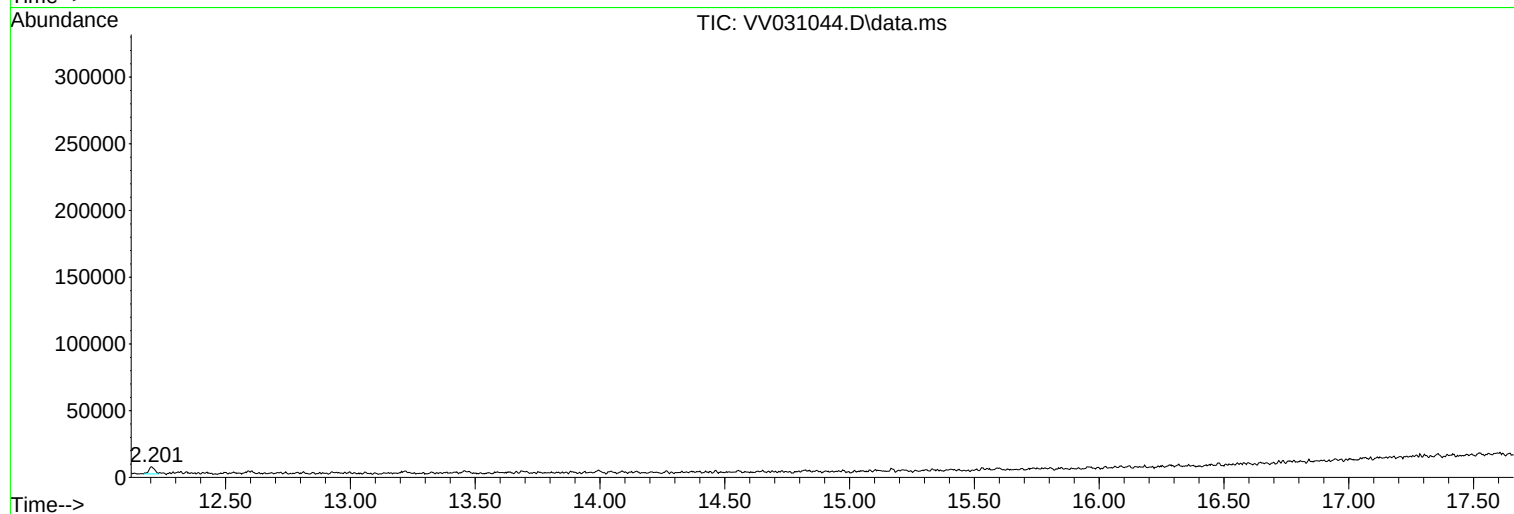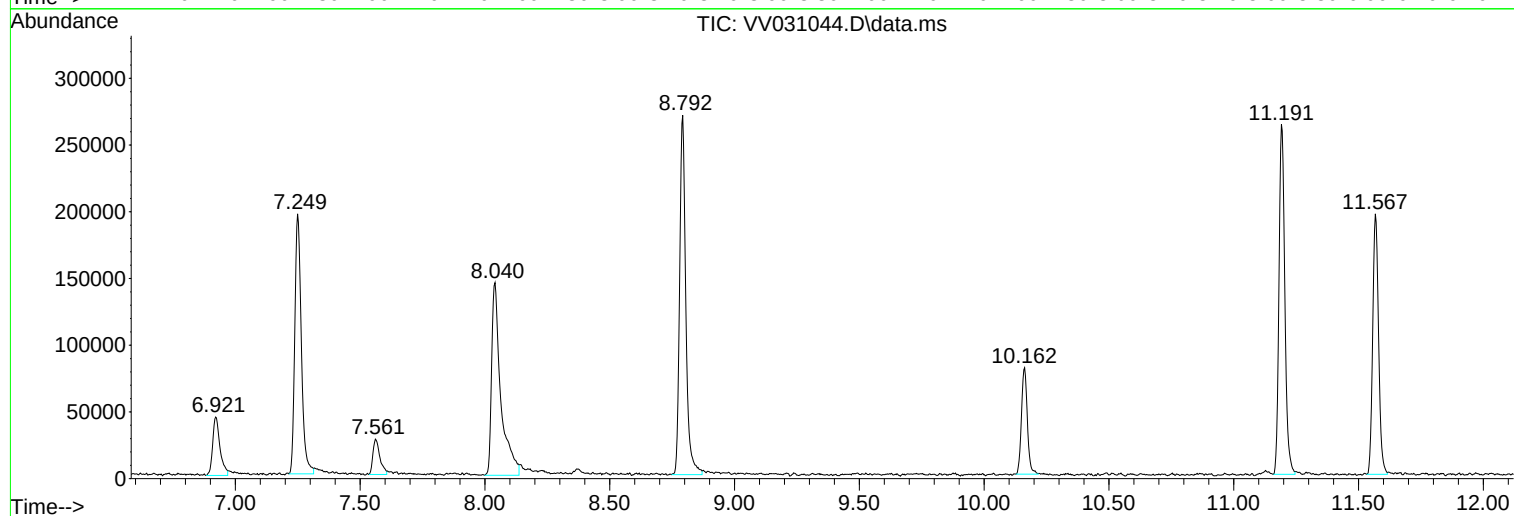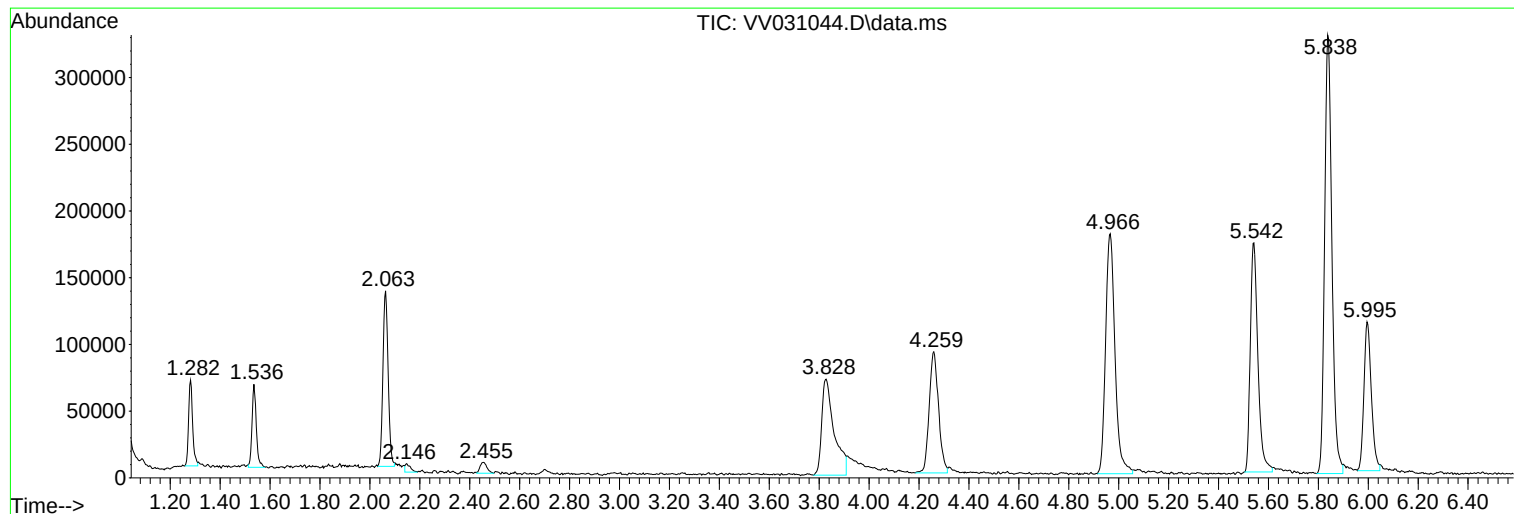

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051623\
Data File : VV031044.D
Acq On : 16 May 2023 11:41
Operator : SY/MD
Sample : 02790-03DL 250X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0NX7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051623\
Data File : VV031044.D
Acq On : 16 May 2023 11:41
Operator : SY/MD
Sample : 02790-03DL 250X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0NX7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc