

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051623\
 Data File : VV031045.D
 Acq On : 16 May 2023 12:05
 Operator : SY/MD
 Sample : 02790-04DL 250X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CONX8DL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV031045.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	87	rBV2	64980	74224	11.08%	1.548%
2	1.536	147	154	163	rBV	61529	71161	10.63%	1.484%
3	2.063	305	318	334	rBV	132270	197317	29.46%	4.116%
4	2.455	429	440	450	rBV2	10973	20129	3.01%	0.420%
5	3.828	852	867	889	rBV4	73057	236618	35.33%	4.936%
6	4.259	983	1001	1028	rBV	89391	239318	35.73%	4.992%
7	4.966	1206	1221	1247	rBV2	185658	483192	72.15%	10.079%
8	5.542	1387	1400	1423	rBV	166986	355647	53.10%	7.418%
9	5.838	1479	1492	1518	rBV	326256	669715	100.00%	13.969%
10	5.998	1528	1542	1560	rBV2	113032	236134	35.26%	4.925%
11	6.921	1815	1829	1849	rBV	44526	92804	13.86%	1.936%
12	7.249	1917	1931	1950	rBV	201815	369846	55.22%	7.714%
13	7.564	2018	2029	2040	rBV2	27504	52276	7.81%	1.090%
14	8.040	2167	2177	2212	rBV	146038	378352	56.49%	7.892%
15	8.793	2399	2411	2432	rBV	255803	438291	65.44%	9.142%
16	10.162	2824	2837	2852	rBV	81453	139466	20.82%	2.909%
17	11.191	3146	3157	3175	rBV	250905	405629	60.57%	8.461%
18	11.567	3260	3274	3290	rBV	198497	325392	48.59%	6.787%
19	12.204	3464	3472	3482	rVB7	5485	8656	1.29%	0.181%




Sum of corrected areas: 4794167

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051623\
Data File : VV031045.D
Acq On : 16 May 2023 12:05
Operator : SY/MD
Sample : 02790-04DL 250X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CONX8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

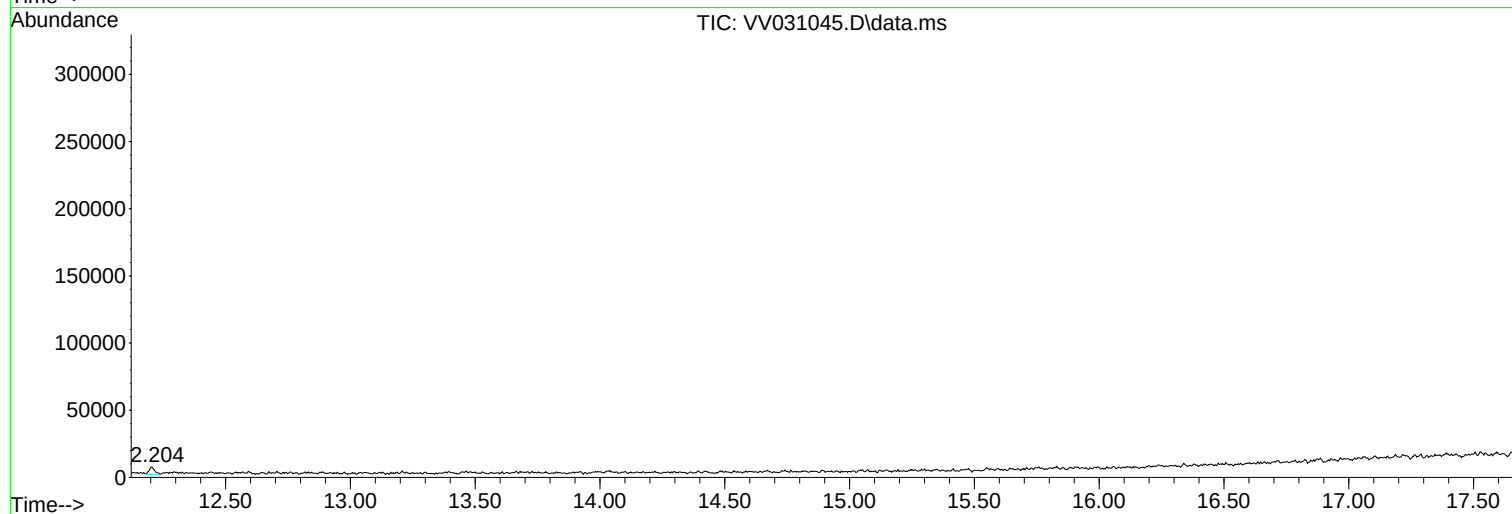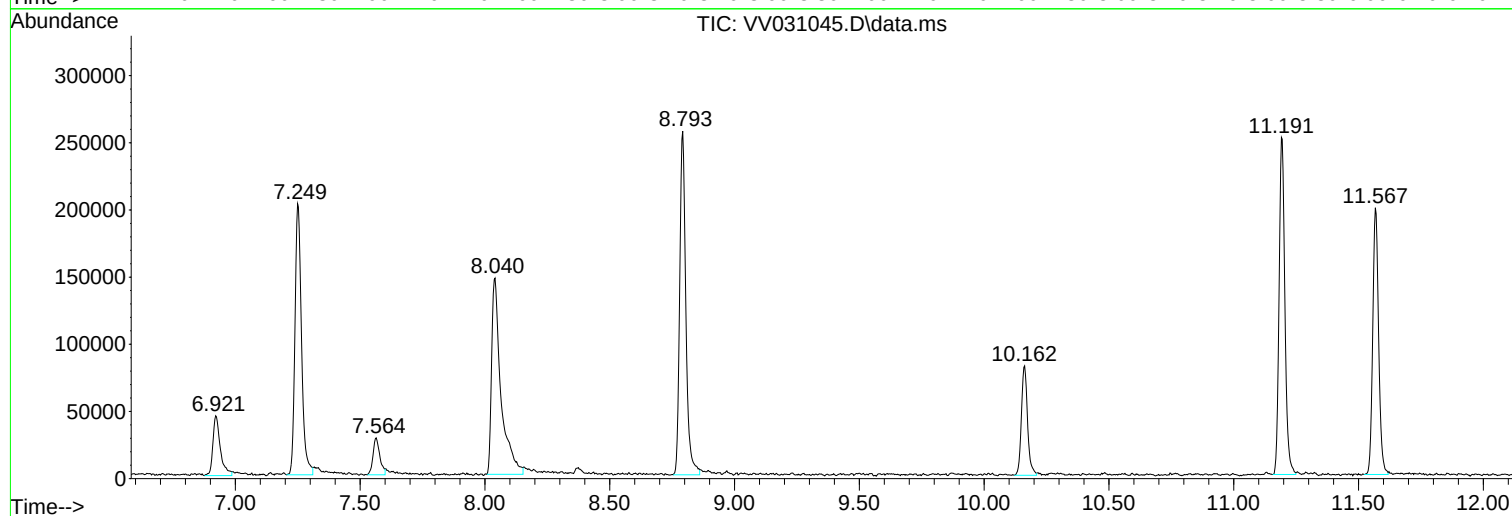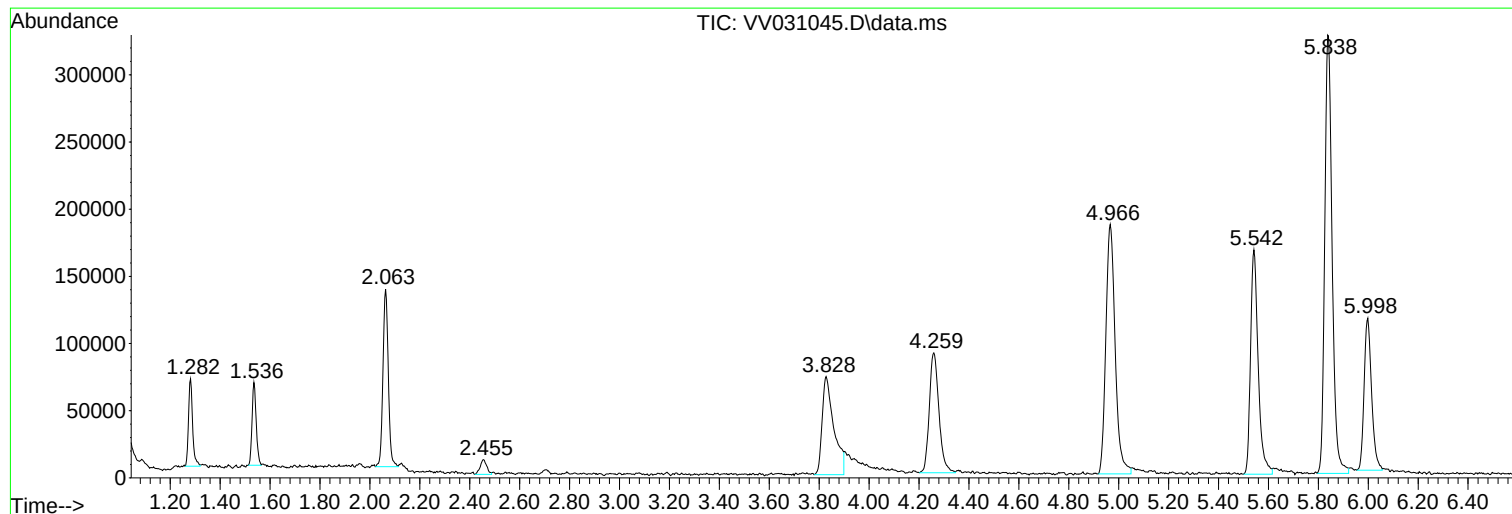

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051623\
Data File : VV031045.D
Acq On : 16 May 2023 12:05
Operator : SY/MD
Sample : 02790-04DL 250X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CONX8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051623\
Data File : VV031045.D
Acq On : 16 May 2023 12:05
Operator : SY/MD
Sample : 02790-04DL 250X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CONX8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc