

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051623\
 Data File : VV031046.D
 Acq On : 16 May 2023 12:28
 Operator : SY/MD
 Sample : 02790-07DL 250X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CONY1DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV031046.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	67	75	91	rVB	68336	75512	12.58%	1.584%
2	1.536	147	154	167	rVB	59851	72903	12.15%	1.530%
3	2.063	306	318	329	rBV	133417	197664	32.94%	4.147%
4	2.455	431	440	452	rVB2	14546	25341	4.22%	0.532%
5	3.828	852	867	906	rBV3	71454	273177	45.52%	5.732%
6	4.259	986	1001	1020	rBV2	89624	234329	39.05%	4.917%
7	4.966	1205	1221	1241	rBV2	190914	493278	82.20%	10.350%
8	5.542	1388	1400	1420	rBV	158195	335285	55.87%	7.035%
9	5.841	1478	1493	1523	rBV	291161	600104	100.00%	12.591%
10	5.998	1530	1542	1566	rVB2	118236	246016	41.00%	5.162%
11	6.921	1818	1829	1844	rBV3	45658	91454	15.24%	1.919%
12	7.252	1918	1932	1948	rBV	204598	377668	62.93%	7.924%
13	7.564	2018	2029	2045	rBV	29461	58709	9.78%	1.232%
14	8.040	2166	2177	2212	rBV	154612	390454	65.06%	8.192%
15	8.793	2397	2411	2431	rBV	249661	418865	69.80%	8.788%
16	10.162	2824	2837	2850	rBV	81270	135336	22.55%	2.840%
17	11.191	3147	3157	3176	rBV	246518	397396	66.22%	8.338%
18	11.567	3260	3274	3292	rBV	205713	333511	55.58%	6.998%
19	12.201	3461	3471	3478	rBV8	5249	9125	1.52%	0.191%




Sum of corrected areas: 4766127

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051623\
Data File : VV031046.D
Acq On : 16 May 2023 12:28
Operator : SY/MD
Sample : 02790-07DL 250X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CONY1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

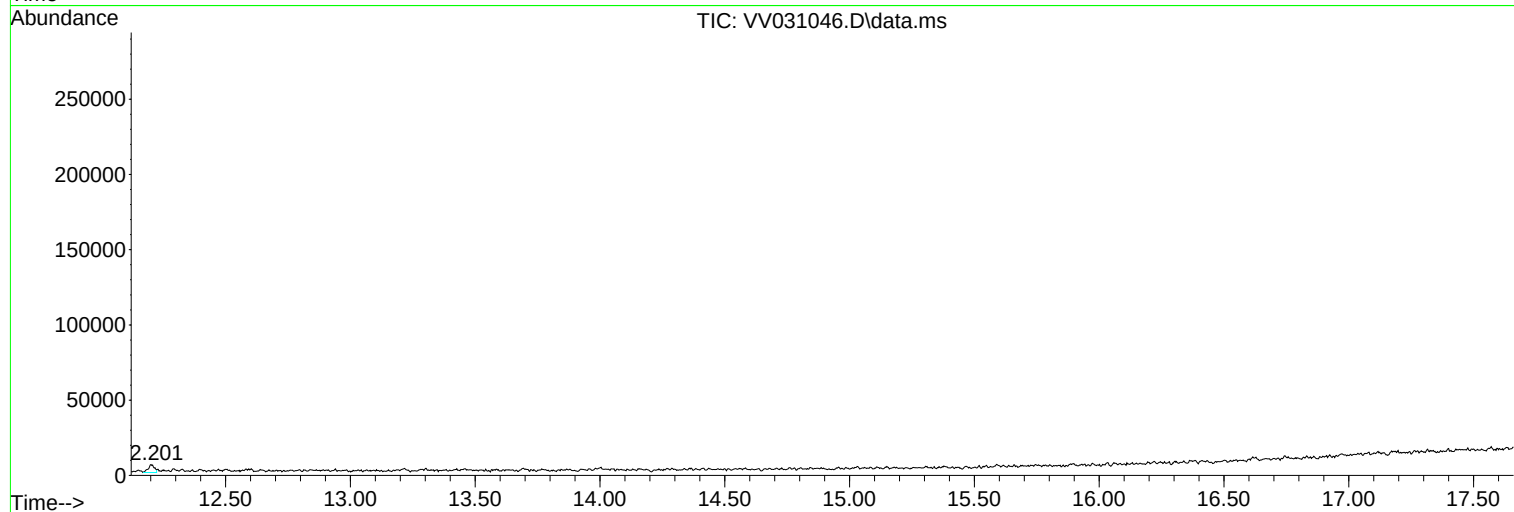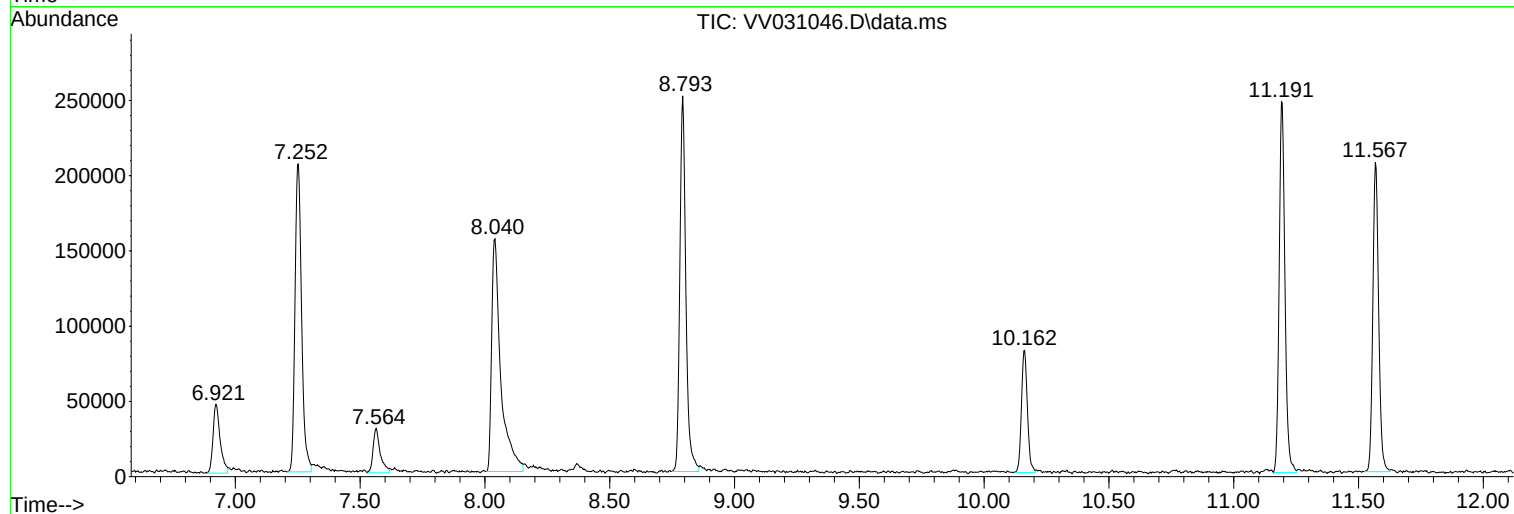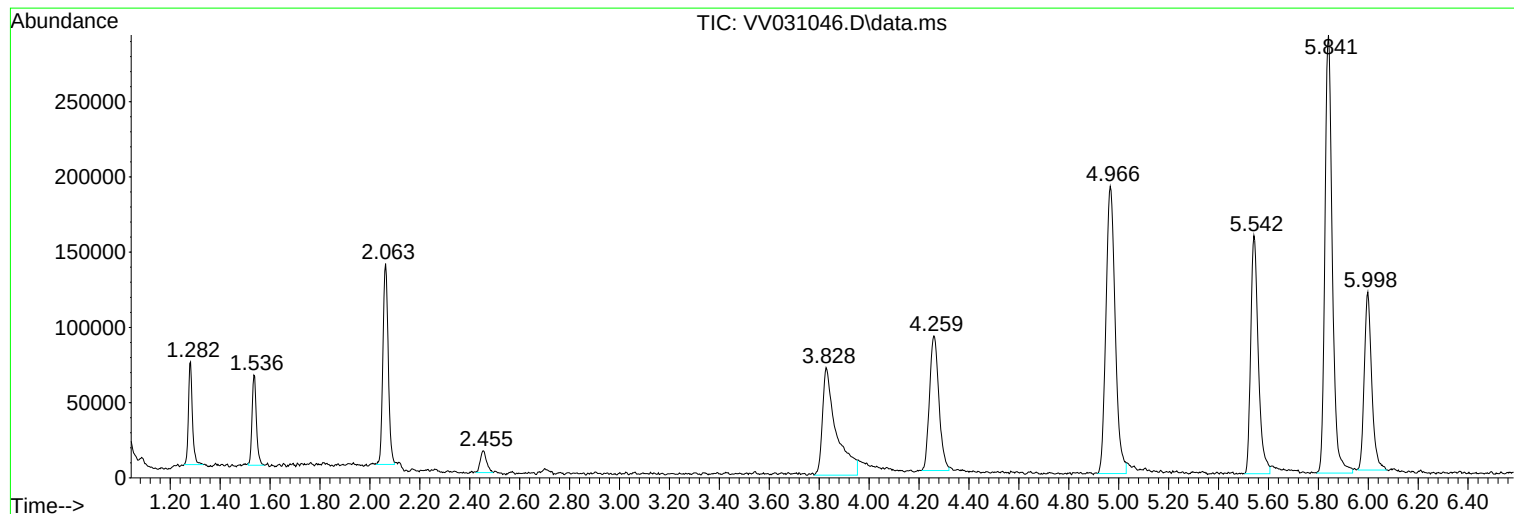

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051623\
Data File : VV031046.D
Acq On : 16 May 2023 12:28
Operator : SY/MD
Sample : 02790-07DL 250X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0NY1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051623\
Data File : VV031046.D
Acq On : 16 May 2023 12:28
Operator : SY/MD
Sample : 02790-07DL 250X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0NY1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc