

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051623\
 Data File : VV031047.D
 Acq On : 16 May 2023 12:53
 Operator : SY/MD
 Sample : 02790-05DL 200X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CONX9DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV031047.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	67	75	89	rBV	64293	74033	15.18%	1.753%
2	1.535	147	154	167	rVB	63777	76642	15.71%	1.815%
3	2.063	307	318	335	rBV	132903	194508	39.88%	4.605%
4	2.455	430	440	448	rBV4	9763	17464	3.58%	0.413%
5	3.828	854	867	885	rBV4	55132	174452	35.77%	4.130%
6	4.259	981	1001	1026	rBV2	91084	240792	49.37%	5.701%
7	4.966	1205	1221	1243	rBV2	192254	487751	100.00%	11.548%
8	5.542	1386	1400	1419	rBV	136273	287823	59.01%	6.814%
9	5.841	1479	1493	1513	rBV	178160	365685	74.97%	8.658%
10	5.998	1528	1542	1564	rBV2	116031	239290	49.06%	5.665%
11	6.921	1819	1829	1845	rBV	44238	86945	17.83%	2.058%
12	7.252	1920	1932	1950	rBV	201420	368434	75.54%	8.723%
13	7.561	2019	2028	2044	rBV2	28269	56855	11.66%	1.346%
14	8.037	2167	2176	2213	rBV	153896	388820	79.72%	9.205%
15	8.368	2272	2279	2284	rBV9	4091	5369	1.10%	0.127%
16	8.792	2401	2411	2428	rBV	205425	351633	72.09%	8.325%
17	10.162	2824	2837	2851	rBV	81112	135981	27.88%	3.219%
18	11.194	3146	3158	3174	rBV	207760	340047	69.72%	8.051%
19	11.567	3262	3274	3291	rVV	203128	331264	67.92%	7.843%




Sum of corrected areas: 4223788

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051623\
Data File : VV031047.D
Acq On : 16 May 2023 12:53
Operator : SY/MD
Sample : 02790-05DL 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CONX9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

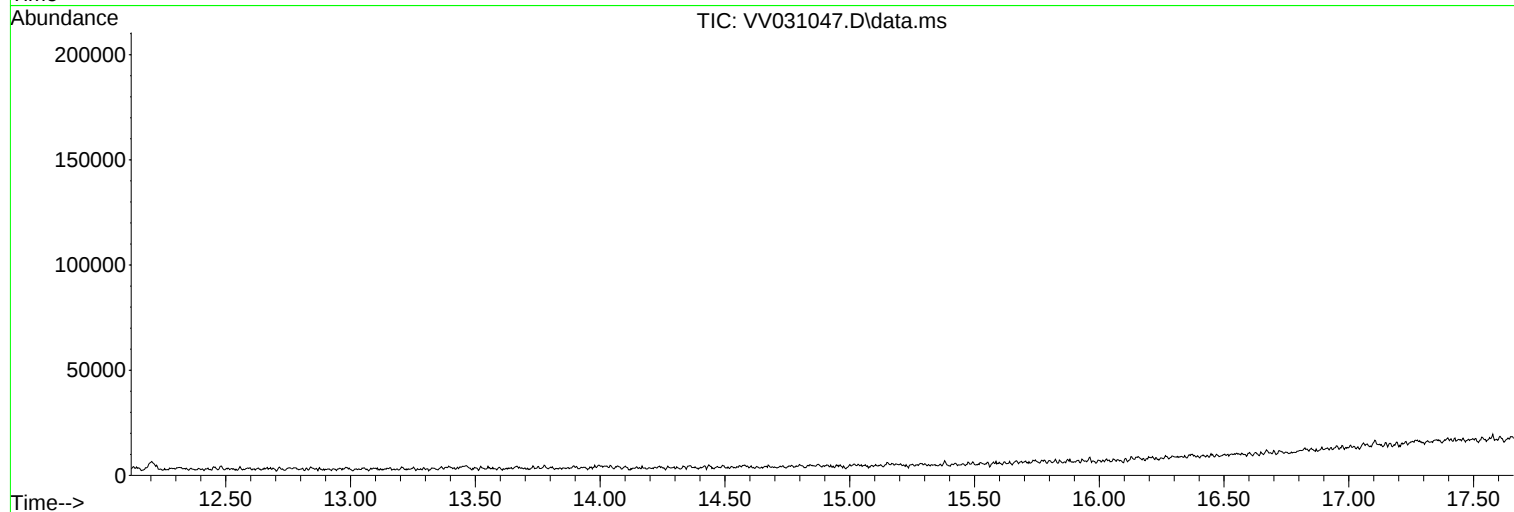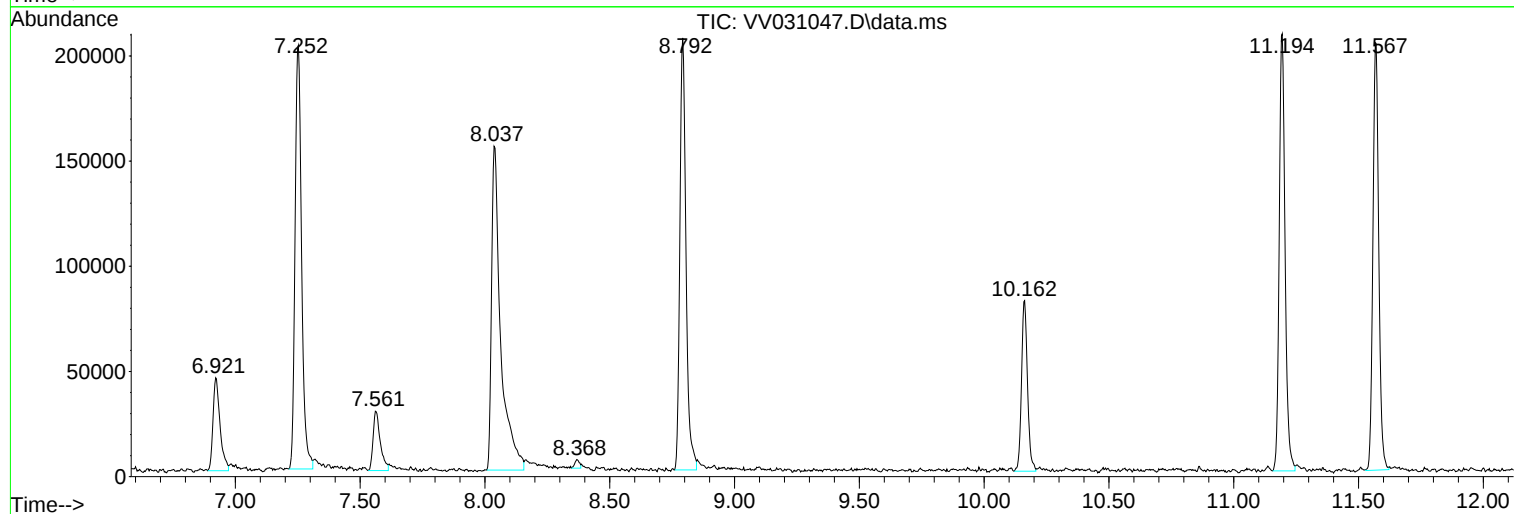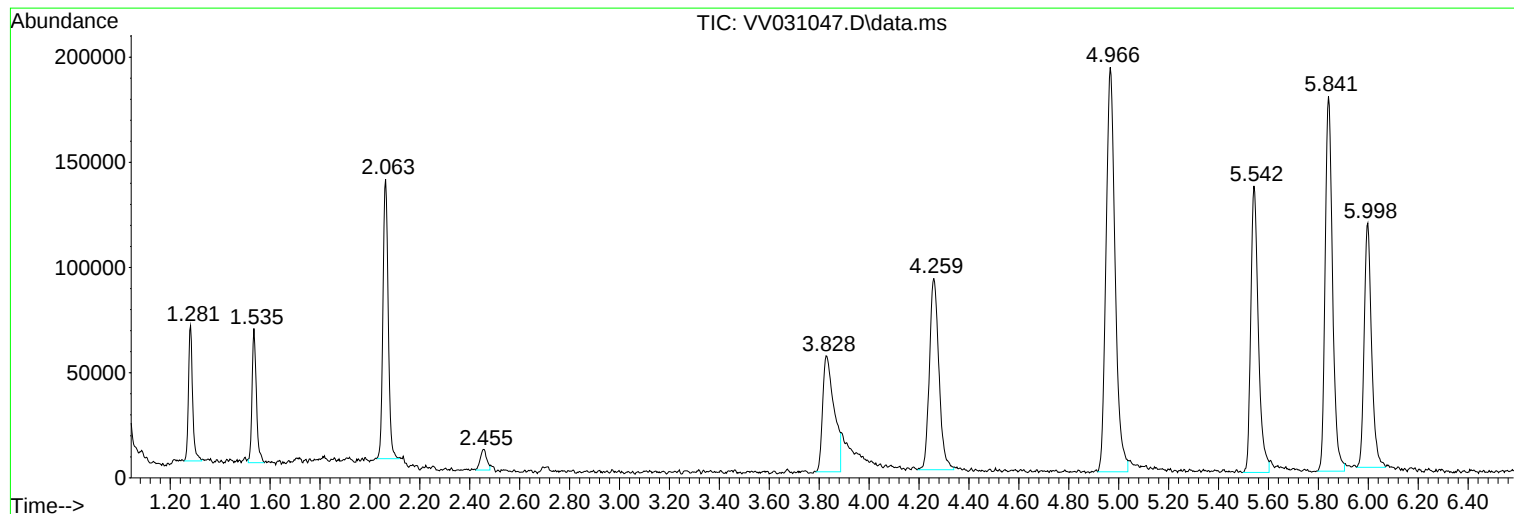

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051623\
Data File : VV031047.D
Acq On : 16 May 2023 12:53
Operator : SY/MD
Sample : 02790-05DL 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0NX9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051623\
Data File : VV031047.D
Acq On : 16 May 2023 12:53
Operator : SY/MD
Sample : 02790-05DL 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0NX9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------