

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051623\
 Data File : VV031048.D
 Acq On : 16 May 2023 13:18
 Operator : SY/MD
 Sample : 02767-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C11F0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV031048.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	87	rBV	57944	65798	12.80%	1.627%
2	1.423	112	119	126	rBV2	17608	20230	3.93%	0.500%
3	1.536	147	154	166	rVB	65026	78703	15.31%	1.946%
4	2.063	309	318	334	rVB	130409	188710	36.70%	4.667%
5	2.455	431	440	448	rBV9	5034	9354	1.82%	0.231%
6	3.822	852	865	892	rBV2	38951	156645	30.47%	3.874%
7	4.259	983	1001	1023	rBV2	96425	253178	49.24%	6.261%
8	4.966	1203	1221	1250	rBV3	196079	514159	100.00%	12.715%
9	5.542	1388	1400	1428	rBV	141282	307473	59.80%	7.604%
10	5.995	1525	1541	1561	rBV3	117155	250932	48.80%	6.206%
11	6.921	1819	1829	1844	rBV	45048	91824	17.86%	2.271%
12	7.252	1920	1932	1950	rBV	206053	377030	73.33%	9.324%
13	7.564	2021	2029	2041	rBV2	28559	51114	9.94%	1.264%
14	8.037	2164	2176	2209	rBV	175263	402614	78.31%	9.957%
15	8.792	2399	2411	2433	rBV	215815	373064	72.56%	9.226%
16	10.159	2824	2836	2851	rBV	85505	141308	27.48%	3.495%
17	10.333	2876	2890	2898	rVB4	6715	11213	2.18%	0.277%
18	11.191	3147	3157	3175	rBV	217298	352357	68.53%	8.714%
19	11.503	3244	3254	3263	rBV3	14708	30696	5.97%	0.759%
20	11.567	3264	3274	3289	rVB	211029	342822	66.68%	8.478%
21	12.294	3492	3500	3510	rBV6	16152	24422	4.75%	0.604%




Sum of corrected areas: 4043646

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051623\
Data File : VV031048.D
Acq On : 16 May 2023 13:18
Operator : SY/MD
Sample : 02767-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C11F0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

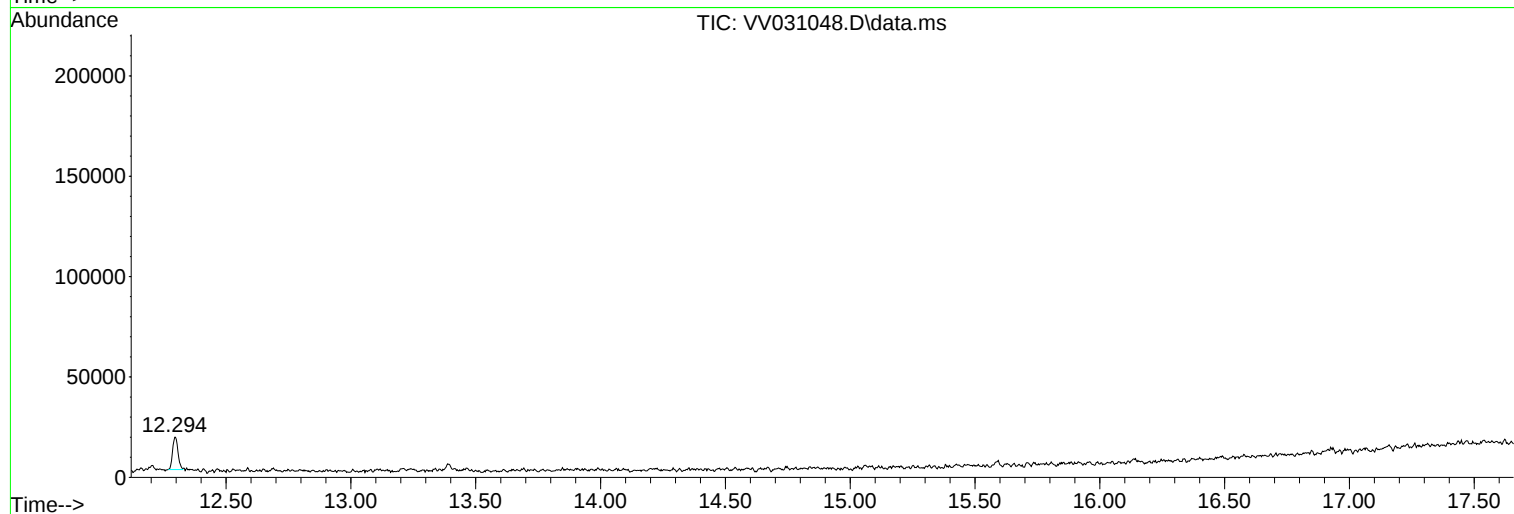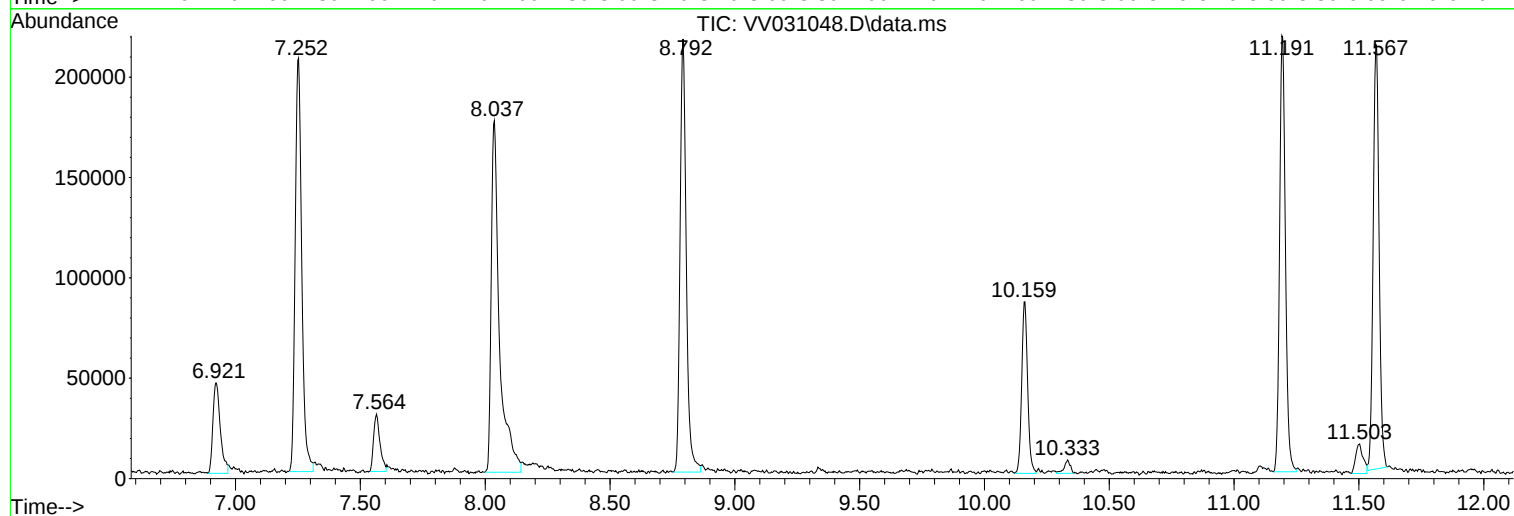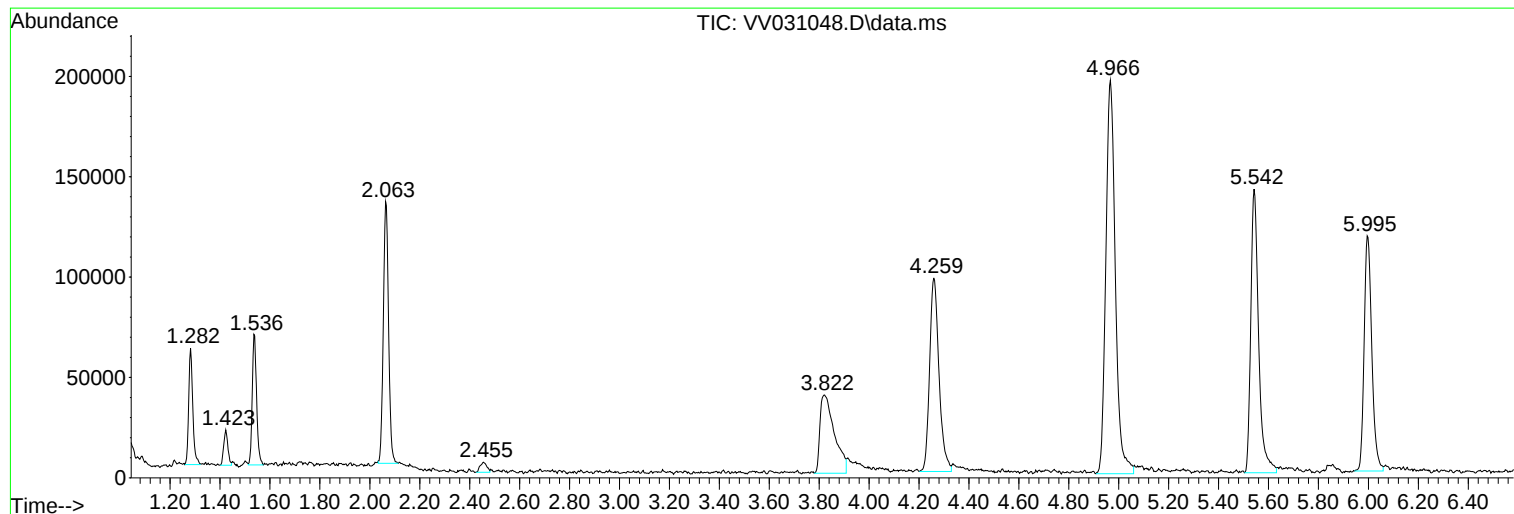

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051623\
Data File : VV031048.D
Acq On : 16 May 2023 13:18
Operator : SY/MD
Sample : 02767-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C11F0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051623\
Data File : VV031048.D
Acq On : 16 May 2023 13:18
Operator : SY/MD
Sample : 02767-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C11F0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
