

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051623\
 Data File : VV031049.D
 Acq On : 16 May 2023 13:42
 Operator : SY/MD
 Sample : 02767-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV031049.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	85	rBV	62250	67916	13.21%	1.650%
2	1.535	147	154	168	rBV	63249	79092	15.38%	1.921%
3	2.063	309	318	334	rVB	139869	204922	39.85%	4.978%
4	2.455	432	440	457	rVB	11640	21634	4.21%	0.526%
5	3.834	857	869	897	rBV2	29596	138671	26.97%	3.369%
6	4.259	985	1001	1026	rVB	97076	253583	49.31%	6.160%
7	4.966	1206	1221	1248	rBV3	198970	514223	100.00%	12.492%
8	5.542	1387	1400	1426	rBV	145827	316382	61.53%	7.686%
9	5.998	1525	1542	1563	rBV	121839	262751	51.10%	6.383%
10	6.921	1817	1829	1850	rBV2	48929	100548	19.55%	2.443%
11	7.249	1917	1931	1952	rBV	215461	399327	77.66%	9.701%
12	7.564	2020	2029	2045	rBV2	28288	54262	10.55%	1.318%
13	7.882	2118	2128	2136	rVB	6244	10615	2.06%	0.258%
14	8.037	2166	2176	2210	rBV	169208	421293	81.93%	10.234%
15	8.792	2398	2411	2434	rBV	226300	392103	76.25%	9.525%
16	10.159	2825	2836	2853	rBV	88242	145231	28.24%	3.528%
17	10.333	2880	2890	2899	rBV3	11877	20426	3.97%	0.496%
18	11.191	3145	3157	3182	rBV	217093	361447	70.29%	8.781%
19	11.567	3262	3274	3294	rBV	207826	343036	66.71%	8.333%
20	12.201	3465	3471	3482	rVB7	5959	8972	1.74%	0.218%




Sum of corrected areas: 4116434

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051623\
Data File : VV031049.D
Acq On : 16 May 2023 13:42
Operator : SY/MD
Sample : 02767-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

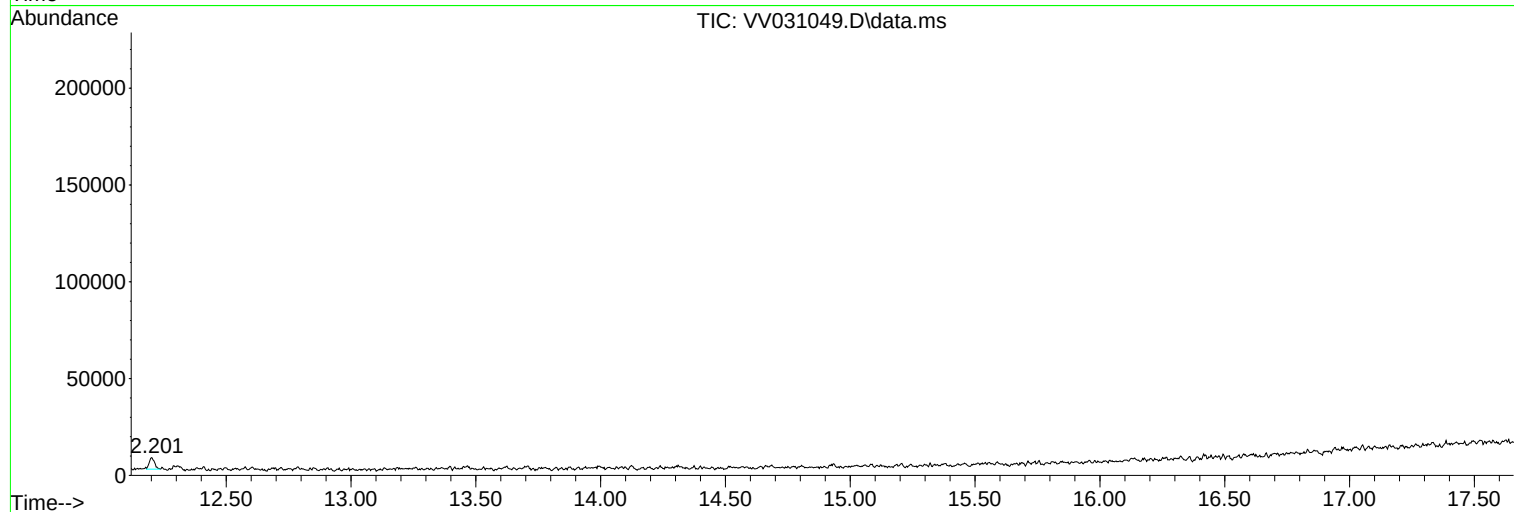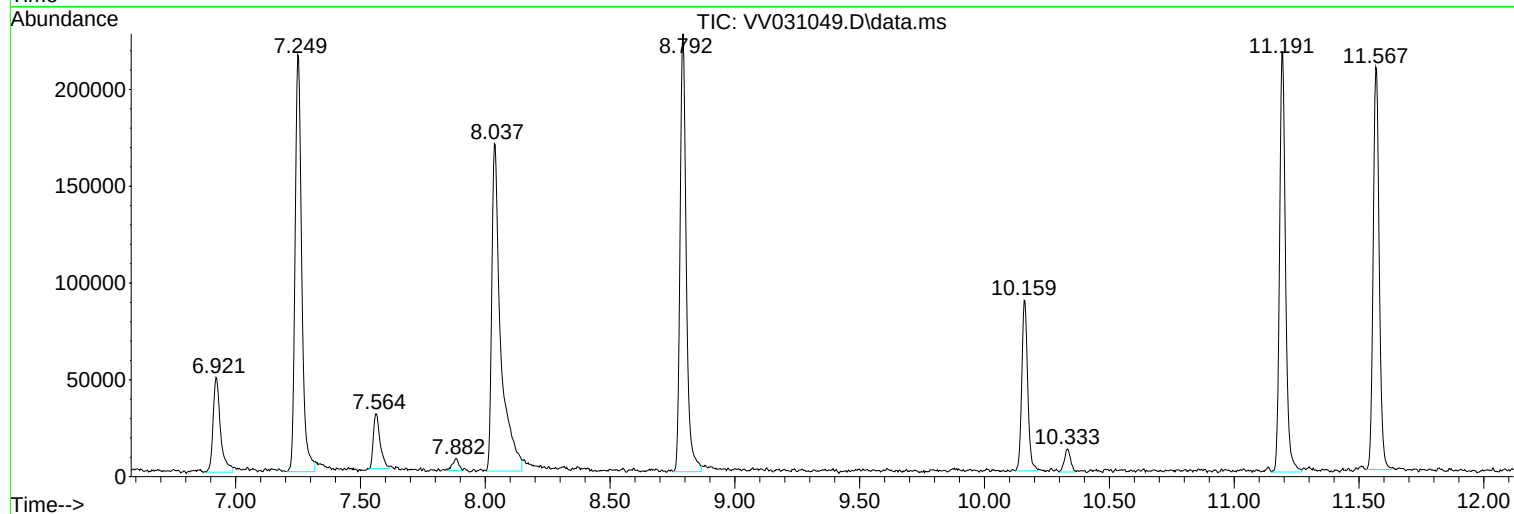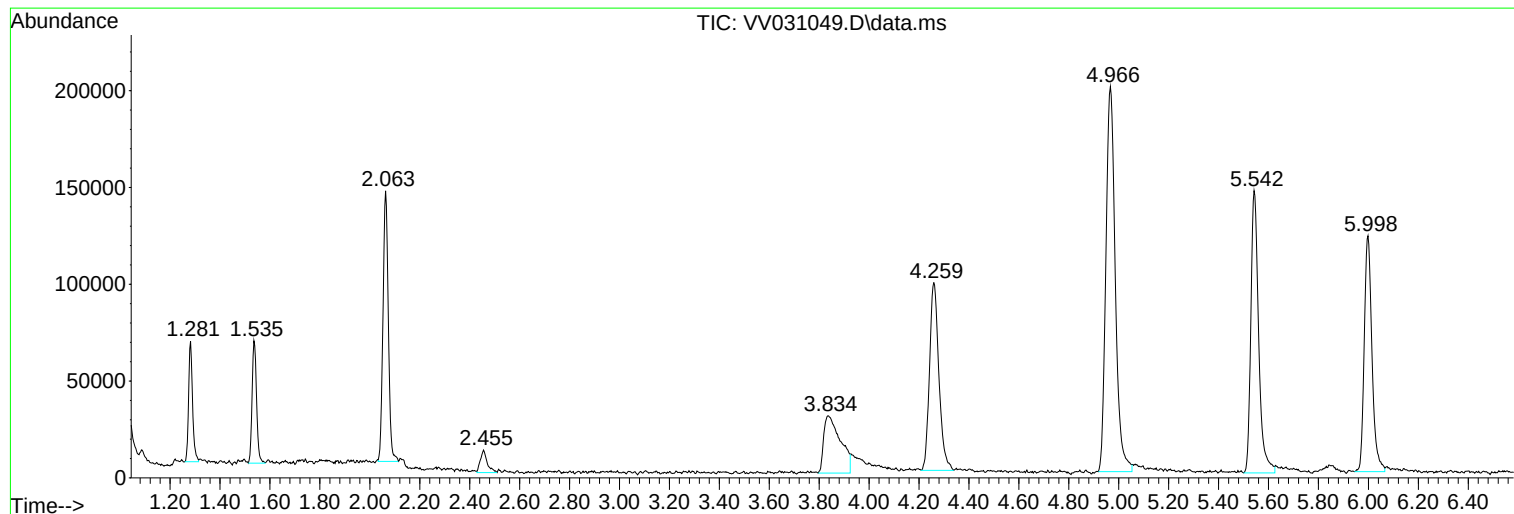

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051623\
Data File : VV031049.D
Acq On : 16 May 2023 13:42
Operator : SY/MD
Sample : 02767-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051623\
Data File : VV031049.D
Acq On : 16 May 2023 13:42
Operator : SY/MD
Sample : 02767-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc