

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051623\
 Data File : VV031050.D
 Acq On : 16 May 2023 14:05
 Operator : SY/MD
 Sample : 02790-06DL 200X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CONY0DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV031050.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	88	rVB	62424	67772	13.92%	1.557%
2	1.539	147	155	170	rVB	60051	74043	15.21%	1.701%
3	2.063	309	318	334	rVB	129220	186459	38.31%	4.284%
4	2.455	431	440	456	rBV3	10869	20146	4.14%	0.463%
5	3.828	854	867	887	rBV3	65452	202708	41.65%	4.658%
6	4.262	987	1002	1023	rBV2	89405	228011	46.85%	5.239%
7	4.966	1204	1221	1246	rBV2	183408	486720	100.00%	11.184%
8	5.545	1388	1401	1425	rBV	144416	311469	63.99%	7.157%
9	5.841	1480	1493	1518	rBV	212198	437264	89.84%	10.047%
10	5.998	1530	1542	1562	rBV2	112679	235579	48.40%	5.413%
11	6.921	1818	1829	1845	rBV	42647	85715	17.61%	1.970%
12	7.252	1918	1932	1946	rBV	198217	362974	74.58%	8.340%
13	7.564	2019	2029	2044	rBV	27498	54516	11.20%	1.253%
14	8.040	2166	2177	2210	rBV	160020	387939	79.70%	8.914%
15	8.371	2270	2280	2287	rBV6	5582	8589	1.76%	0.197%
16	8.793	2399	2411	2435	rBV	218682	383377	78.77%	8.809%
17	10.162	2826	2837	2851	rBV2	82294	133139	27.35%	3.059%
18	11.194	3145	3158	3175	rBV	218713	355468	73.03%	8.168%
19	11.567	3262	3274	3287	rBV	196837	322636	66.29%	7.413%
20	12.204	3460	3472	3478	rBV	4454	7582	1.56%	0.174%




Sum of corrected areas: 4352106

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051623\
Data File : VV031050.D
Acq On : 16 May 2023 14:05
Operator : SY/MD
Sample : 02790-06DL 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CONY0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

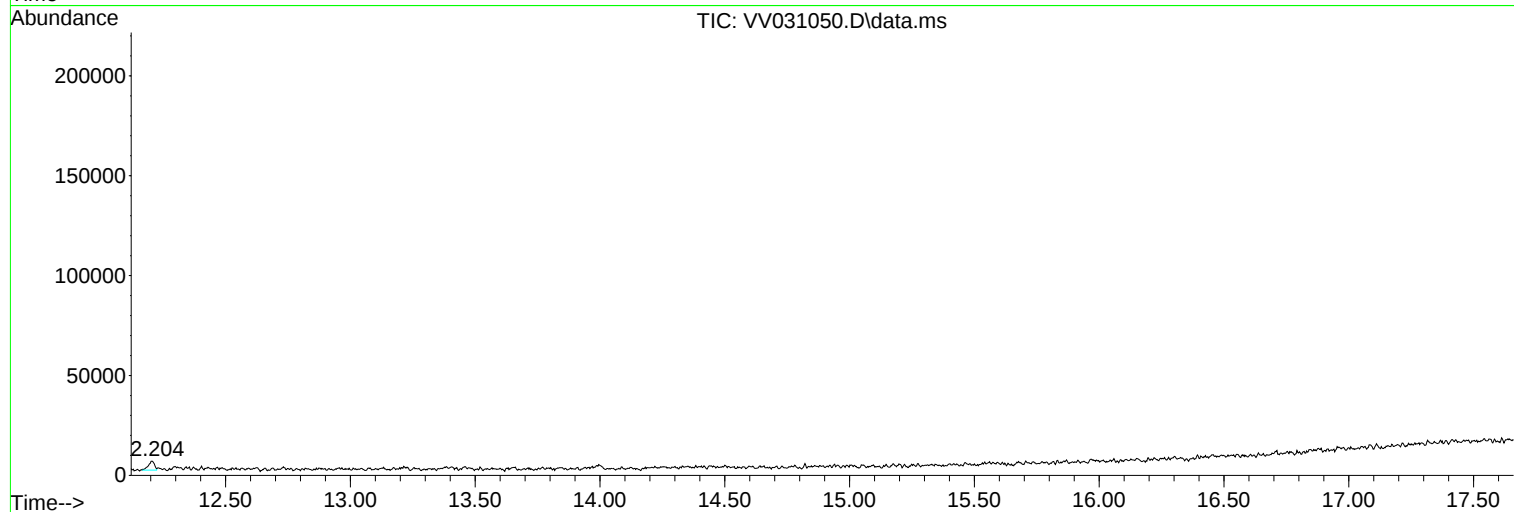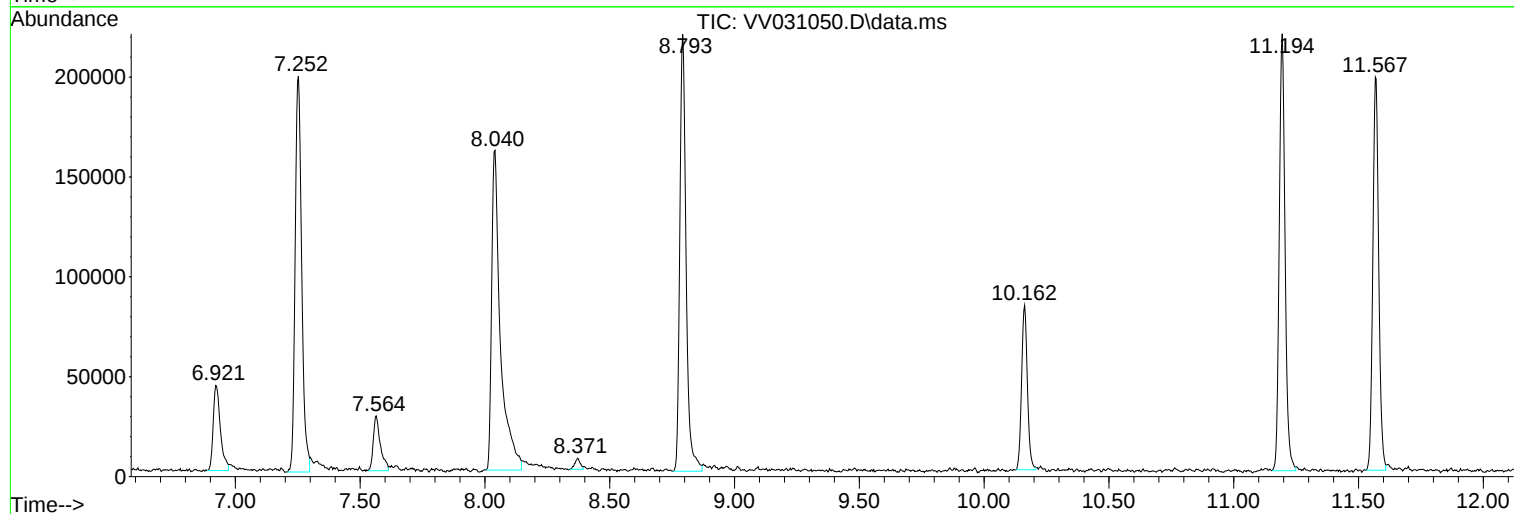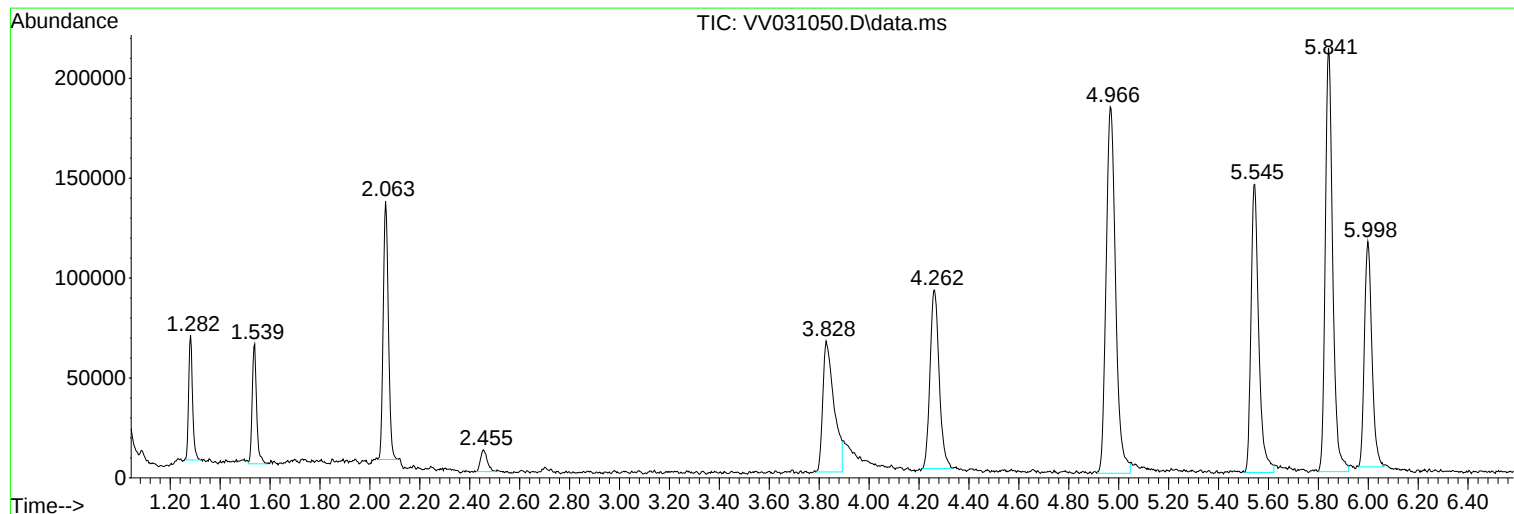

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051623\
Data File : VV031050.D
Acq On : 16 May 2023 14:05
Operator : SY/MD
Sample : 02790-06DL 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0NY0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV051623\
Data File : VV031050.D
Acq On : 16 May 2023 14:05
Operator : SY/MD
Sample : 02790-06DL 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0NY0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc